

USER MANUAL



MPW-352
MPW-352R
MPW-352RH

Read before use!

Device serial number:

For centrifuges with serial no (SN):

MPW-352 10352150724 – ...

MPW-352R 10352R137323 – ...

MPW-352RH 10352RH014524 – ...



This manual was prepared with special care. MPW MED. INSTRUMENTS may change the manual at any time and without notice because of improvements, typographical errors or improvements to facilities
All rights reserved. No part of this User Manual may be modified, distributed, published or reproduced without the prior permission of MPW MED. INSTRUMENTS.

You can find the current version of the user manual on our website under:

mpw.pl/en – DOWNLOAD section (one can choose demanded language version of website).

Content

1 Symbols and designations	5
1.1 Designations used in the manual	5
1.2 Markings on the device	5
1.3 Markings on the packaging	6
2 Application	6
3 Technical specification	7
3.1 Environmental conditions	7
4 Installation	8
4.1 Content of the package	8
4.2 Location selection	8
4.3 Preparation for installation	9
4.4 Unpacking the device	10
4.5 Centrifuge installation	10
4.6 First start of the centrifuge	10
4.7 Turning on the centrifuge	10
4.8 Turning off the centrifuge	10
4.9 Opening and closing the cover	10
4.10 Current protection	11
5 Safety notes	11
5.1 General remarks	11
5.2 Placing the rotor and accessories in the centrifuge	11
5.3 Filling tubes	12
5.4 Filling the rotor	13
5.5 Safety hints	14
5.6 Operating conditions	15
5.7 Equipment life	16
5.8 Service life of rubber suspension components of the drive unit	16
5.9 Work safety	17
5.10 Unbalance	17
5.11 Emergency stop	18
5.12 Residual risk	18
5.13 Obligation to report a serious device incident	18
6 Product description	19
6.1 Product Design and Appearance	19
6.2 Name plate	20
6.3 Control device	20
6.4 Setting parameters	20
6.5 Safety features	20
6.6 Increase in temperature (MPW-352 only)	21
7 Centrifuging	22
7.1 Control panel	22
7.2 Display	22
7.3 Setting up RPM, RCF, time, temperature	24
7.4 Users programs	25
7.5 Creator of acceleration and deceleration curves	27
7.6 Programs with user characteristics	30
7.7 Rotor choosing	31
7.8 SHORT mode	31
7.9 Finishing the centrifuging	31
7.10 Temporarily disabled functions	32
8 Temperature control	32
8.1 Initial cooling during centrifuging –FAST COOL	32

8.2 Initial cooling or heating without centrifuging – THERMAL CHAMBER	33
8.3 Cooling or heating in “START DELAY – OF TEMPERATURE” mode	33
8.4 Cooling or heating in „SHORT” mode	33
8.5 Cooling and heating notes	33
9 Parameters of centrifugation	34
9.1 Acceleration/deceleration – changing characteristics	34
9.2 Radius	35
9.3 Sample density	35
9.4 Temperature offset	35
9.5 Thermal chamber	36
9.6 Automatic lid opening	37
9.7 Start delay - of time	37
9.8 Start delay – of temperature	38
10 Menu	38
10.1 Screen saver	39
10.2 Visual alarm	39
10.3 Types of main screen	39
10.4 Rotating runtime	40
10.5 Buzzer	41
10.6 Date/time	41
10.7 Language	41
10.8 Other	42
10.9 Password	43
10.10 Last 10 cycles	45
10.11 Work time	45
10.12 Rotor runtime	45
10.13 Contact us	45
10.14 Diagnostics	46
10.15 Factory settings	46
11 Maintenance	46
11.1 Cleaning of the centrifuge	46
11.2 Maintenance of centrifuge elements	46
11.3 Sterilization	47
11.4 Chemical resistance	49
12 Troubleshooting	50
12.1 Messages	50
12.2 Emergency cover release	51
13 Guarantee	51
14 Transport and storage	52
14.1 Transport and storage conditions	52
15 Disposal	52
16 List of changes in the manual	53
17 Manufacturer’s info	54
18 Distributor’s info	54
19 Annexes	54
A. Additional accessories	
B. Declaration of conformity (CE, ROHS 2)	
C. Declaration of decontamination (repair / return)	
D. Nomogram RPM / RCF	

1 Symbols and designations

1.1 Designations used in the manual

	WARNING! General hazards		Symbol for identifying an in vitro diagnostic medical device
	WARNING! Risk of crushing injury		CE mark
	DANGER! Risk of electric shock		Symbol indicating disposal method
	DANGER! Biological hazard		Please read the instruction manual before using the device
	DANGER! Risk of explosion with possible serious injury or death		Manufacturer information

1.2 Markings on the device

Symbol	Explanation	Location
	Information about the direction of rotation of the rotor	Under the centrifuge lid
	Information on where and how to use the emergency lid opening mechanism	On the side of the centrifuge next to the emergency opening of the lid
 Uwaga! Przed awaryjnym otwarciem pokrywy, wyłączyc urządzenie i odłączyć kabel zasilający. Odczekaj 10 min i/lub zaglądając przez wziernik, upewnić się, że wirnik nie obraca się, a następnie otworzyć pokrywę. Attention! Before emergency opening the cover, switch off the mains power switch and disconnect the power cord. Wait 10 min and/or looking through the sight glass, make sure that the rotor is not rotating.	Information about the place of danger	On the side of the centrifuge next to the emergency opening of the lid
	Reminder for proper rotor maintenance	Under the centrifuge lid

		Information about correct and incorrect filling of rotors	Under the centrifuge lid
	 Tighten the rotor fixing screw with the provided key. Dokręcić śrubę mocującą wirnik za pomocą dostarczonego klucza.	Information reminding about the proper tightening of the rotor screw	Under the centrifuge lid

1.3 *Markings on the packaging*

REF	Device catalog number		Maximum number of pieces in a stack
SN	Serial number of the device		Temperature limit
	Date of manufacture of the device		Humidity limit
	Manufacturer's data		CE mark
	Delicate, handle with care!		Green dot
	Protect from moisture!		Packaging made of recyclable materials
	Top of the load		

2 Application

- **MPW-352/R/RH** centrifuges are a family of table-top non-automatic laboratory centrifuges (**MPW-352** – ventilated centrifuge, **MPW-352R** – refrigerated centrifuge, **MPW-352RH** – refrigerated and heated centrifuge).
- The devices are intended for In Vitro Diagnostics (IVD). This means that it is an in vitro diagnostic medical device - in accordance with the 2017/746 Regulation of the European Parliament and of the Council (EU) of 5 April 2017 on in vitro diagnostic medical devices and repealing Directive 98/79/EC and Commission Decision 2010 /227/EU.
- Centrifuges are used to separate aqueous solutions and suspensions of samples with a density not higher than **1.2g/cm³** taken from human, animal and plant organisms into components of different densities under the influence of centrifugal force, in order to provide information about their biological state and to other analytical work.

- The design of the centrifuge ensures ease of use, safe operation and a wide range of applications in medical, biochemical and other analysis laboratories.
- The centrifuge is not biotight, therefore, when centrifuging preparations that require biotightness, containers and rotors with a biotightness certificate should be used.

3 Technical specification

manufacturer	'MPW MED. INSTRUMENTS' SPÓŁDZIELNIA PRACY, Bořemlowska 46 Street, 04-347 Warsaw																																													
type	MPW - 352					MPW - 352R					MPW - 352RH																																			
cat. number (REF)	10352/2-56	10352/1-56/100	10352/1-56/110	10352/1-56	10352/1-56/127	10352R/2-5	10352R/2-6	10352R/1-6/100	10352R/1-6/110	10352R/1-6	10352R/1-6/127	10352RH/2-5	10352RH/2-6	10352RH/1-6/100	10352RH/1-6/110	10352RH/1-6	10352RH/1-6/127																													
mains voltage [V] (L1+N+PE)	230	100	110	120	127	230	230	100	110	120	127	230	230	100V	110	120	127																													
	±10%	±5%			±10%		±5%			±10%		±5%			±5%																															
mains frequency [Hz]	50/60				50	60	60				50	60	60																																	
power consumption (max.)	500W				1000W				1100W																																					
current protection [A]	T6,3A	T10A			T10A		-			T10A		-																																		
cooling medium	-				R452A																																									
capacity (max.)	1000 ml																																													
speed – RPM	90 ÷ 18000 rpm (step 1 x g)																																													
force – RCF	24270 x g (step 1 x g)				30065 x g (step 1 x g)																																									
kinetic energy (max.)	14000 J																																													
running time time counting short-time operation mode – SHORT continuous operation mode – HOLD	00:00:01 ÷ 99:59:59 – [hours, min., sec] (step 1s) since start button is pressed / since preselected speed is reached																																													
yes																																														
yes																																														
Menu languages	Polish, English, German, Spanish, Italian, Portuguese, Russian, Swedish, French, Czech																																													
user programs	100																																													
adjustable temperature	-				-20 ÷ 40°C* (step 1°C)					-20 ÷ 55°C* (step 1°C)																																				
pre-cooling/heating	no/no				yes/no					yes/yes																																				
guaranteed temperature with max. rotor speed	-														$\leq 4^{\circ}\text{C}$																															
cooling/heating without centrifuging	no				yes/ no					yes / yes																																				
cooling/heating with centrifuging	no				yes / no					yes / yes																																				
acceleration (ACEL)	10 linear curves																																													
deceleration (DECEL)	10 linear curves																																													
programmable non-linear curves: acceleration deceleration	10																																													
acceleration	10																																													
USB communication	no																																													
Electromagnetic compatibility	according to EN 61326-2-6:2006																																													
degree of protection (according to PN-EN 60034-5:2021-01)	IP21					IP20																																								
height (H)	380 mm				380 mm				443 mm				443 mm																																	
width (W)	443 mm				545 mm				695 mm				768 mm																																	
depth (D)	545 mm				768 mm				768 mm																																					
height with open cover (H _{oc})																																														
noise level	<65 dB																																													
weight 230V	ok. 42 kg				ok. 65 kg				ok. 66 kg																																					
weight 120V	ok. 45 kg				ok. 69 kg				ok. 70 kg																																					

*Time and possibility of obtaining a set temperature is dependent on multiple factors , including rotor type, established RPM, ambient temperature; accuracy: ± 1°C (for 352R), ± 3°C (for 352RH) appropriate for place of temperature sensor

3.1 Environmental conditions

- The device may only be used indoors.

- The permissible ambient temperature is 2°C to 40°C.
- Maximum allowed relative humidity 80% at temperature up to 31°C decreasing linearly to 50% relative humidity at 40°C.
- The mains voltage fluctuations must not exceed $\pm 10\%$ of the nominal voltage.
- Maximum altitude 2,000 m above sea level.
- Overvoltage category II.
- Pollution degree 2.

4 Installation

4.1 Content of the package

name	pcs.	cat no. (REF)	
Centrifuge MPW-352/R/RH (type and supply version dependent)	1	10352/2-56; 10352/1-56; 10352/1-56/100; 10352/1-56/110; 10352/1-56/127; 10352R/2-5; 10352R/2-6; 10352R/1-6; 10352R/1-6/100; 10352R/1-6/110; 10352R/1-6/127 10352RH/2-5; 10352RH/2-6; 10352RH/1-6; 10352RH/1-6/100; 10352RH/1-6/110; 10352RH/1-6/127	
Rotor fixing screw	1	17664	
rotor key	1	17665	
key for emergency lock release	1	17162	
power cord -MPW-352/R/RH 230V -MPW-352 120V -MPW-352R/RH 120V	1	17866 17867 17010	
fuse WTAT 6,3A 250V (for MPW-352 230V) / WTA T10A 250V (for MPW-352 120V and MPW-352R/RH 230V) / without fuse (for MPW-352R/RH 120V)	2	17862 17863 none	
Vaseline 20ml	1	17201	
user manual	1	See page 1	

4.2 Location selection

	WARNING! Risk of damage to the device. <ul style="list-style-type: none"> The table intended for the centrifuge operation should be adapted to the weight of the device, clean, stable and free from vibrations, and have a flat, levelled top.
---	---

	<ul style="list-style-type: none"> ▪ In accordance with the EN 61010-2-020 standard, leave a safety distance of 30 cm from the operating device. Keep a distance from walls and other devices. Do not place any objects in this area. ▪ The centrifuge should be positioned so that access to the mains switch is not difficult. ▪ Do not use the device near strong, unshielded, high-frequency electromagnetic sources as they may interfere with its proper operation. ▪ Do not install the centrifuge near heat sources (e.g. radiators). ▪ Avoid direct sunlight. ▪ Ensure adequate ventilation of the room. ▪ During centrifugation, it is forbidden to stay in the safety zone, i.e. 30 cm distance around the centrifuge, or to leave objects, e.g. glassware, inside this zone. ▪ It is forbidden to place any objects on the centrifuge. ▪ Never use the centrifuge on trolleys or on single stands if they may start to move during operation or are inappropriate for the size of the centrifuge.
--	--

4.3 Preparation for installation

	<p>WARNING! Risk of injury or damage to the device.</p> <ul style="list-style-type: none"> ▪ Lifting and moving the device can cause injuries due to its heavy weight. ▪ A sufficient number of people (min. 2) should be used to lift and transport the centrifuge. ▪ Lift the device from the bottom near its feet. Do not grab it by the front panel. ▪ After changing the storage location of the device (from cold to warm), wait until the device has warmed up to the ambient temperature to avoid damage to the electronic components or compressor failure due to condensation. ▪ It is important to allow sufficient time for the device to dry before restarting it (min. 4 hours).
--	--

	<p>WARNING! Risk of electric shock or fire.</p> <ul style="list-style-type: none"> ▪ The centrifuge may only be operated in a building that complies with applicable national regulations and standards. In particular, it must be ensured that power supply circuits located upstream of the device's internal protection are not loaded in an unauthorized manner. This can be ensured by using additional interrupters or other suitable fuse elements in the building installation. ▪ The voltage and frequency of the power source must comply with the requirements specified on the device nameplate. ▪ The power socket must be earthed with a protective conductor (PE). ▪ During operation, there must be easy access to the power switch and the device that cuts off the electrical network (e.g. residual current device). ▪ Only use the power cord supplied with the centrifuge. ▪ Before turning on the device, make sure it is properly connected to the power source.
--	---

4.4 Unpacking the device

- 1) Open the package.
- 2) Remove the box containing the accessories.
- 3) Remove the centrifuge from the box and remove the foil (keep the packaging and packing material for service shipment).
- 4) Make sure that all the items are included in the package (table in the "Package contents" section).
- 5) Place the device on a suitable laboratory table.

4.5 Centrifuge installation

- 1) Check whether the mains voltage and frequency meet the requirements given on the nameplate of the device.
- 2) Connect the power cord to the centrifuge power socket (on the rear wall of the centrifuge) and to the power source.

4.6 First start of the centrifuge

- 1) Wait at least 4 hours for the unit to reach ambient temperature to avoid compressor failure or damage to electronic components due to condensation.
- 2) Turn on the centrifuge power using the mains switch located on the side wall of the device.
- 3) Open the cover according to the section ***Opening and closing the cover***.
- 4) Install the rotor according to the section ***Placing the rotor and accessories in the centrifuge***.
- 5) Set centrifugation parameters according to the sections ***Centrifuging*** and ***Parameters of centrifugation***.

4.7 Turning on the centrifuge

To turn on the centrifuge, set the mains power switch to position 1. After the start-up process is complete, the centrifuge is ready to operate.

4.8 Turning off the centrifuge

Prerequisites:

- The centrifugation cycle is complete.
- The device cover is open.

- 1) Turn off the device using the mains power switch located on the side wall of the device.

4.9 Opening and closing the cover

	ATTENTION ! <ul style="list-style-type: none">▪ The cover can only be opened when the centrifuge is at rest (the rotor is not rotating).▪ Centrifugation can only be started with the lid closed.
	WARNING! Risk of injury. <ul style="list-style-type: none">▪ Do not put your hands between the cover and the housing when closing the centrifuge cover.

- 1) Press the **COVER** button  to open the cover.
- 2) To close the lid, press it down with both hands until the lock engages.

4.10 Current protection



Centrifuges MPW-352/R/RH 230V and MPW-352 120V are equipped with a current protection (melting fuse) located in the mains power socket on the rear wall of the centrifuge, while the MPW-352R/RH 120V centrifuges have thermal protection (without an additional fuse).

5 Safety notes

5.1 General remarks



- The laboratory centrifuge may be operated only by qualified laboratory personnel, after reading the operating manual.
- The operating instructions are part of the product.
- The operating manual should always be kept in the vicinity of the centrifuge.
- The centrifuge cannot be operated contrary to its purpose.
- If the centrifuge is used in a manner inconsistent with the manufacturer's guidelines, the safety of its use may be impaired.
- For centrifugation in the centrifuge, only containers and inserts provided in the list of equipment and centrifuge tubes, the diameter, length and strength of which are appropriate, should be used. The use of test tubes not included in the list should be agreed with MPW MED. INSTRUMENTS or its authorized representatives.
- Pay attention to the quality and appropriate thickness of the glass test tubes walls. Glass tubes should be centrifuge tubes, and their use in the centrifuge should be made dependent on the following guidelines:

glass tubes	max RCF in angular rotors	max RCF in horizontal rotors
5-10 ml	3000 x g	4000 x g
30-100 ml	spinning not allowed	4000 x g

- Weighing the filled test tubes into the rotor is recommended. When centrifuging in horizontal rotors, it is recommended to weigh the filled containers / hangers. This will allow to minimize the differences in mass between them, and as a result to avoid the negative impact of vibrations on the engine suspension and to reduce noise levels during the operation of the centrifuge.

5.2 Placing the rotor and accessories in the centrifuge




- Connect the centrifuge to the power supply (mains socket at the back of the centrifuge).
- Turn on the centrifuge (switch on the side of the centrifuge).
- Open the cover of the centrifuge by pressing the COVER key. Before installing the rotor, check that the rotating chamber is free from any contamination. If there is dust, glass splinters, liquid residues, etc., remove them.
- The rotor can fall if not handled properly, therefore it should always be handled and placed in the centrifuge using both hands.
- Place the rotor on the motor axis by sliding it onto the cone as far as it will go (keeping the coaxiality between the rotor and the motor axis).
- Screw the screw fixing the rotor into the motor axis (clockwise), and then tighten it firmly with the rotor key.
- Fill the rotor with containers / hangers / test tubes according to recommendations in section **Filling the rotor**.


- | | |
|--|--|
| | <ul style="list-style-type: none"> In order to replace the rotor, first remove the tubes and containers from it, unscrew the screw fixing the rotor with the enclosed rotor key, counterclockwise, then using both hands, grab the rotor on opposite sides and remove it from the motor axis. Install another rotor as described above instructions. |
|--|--|

5.3 Filling tubes

- | | |
|--|---|
| | <ul style="list-style-type: none"> Fill test tubes outside the centrifuge. |
|--|---|

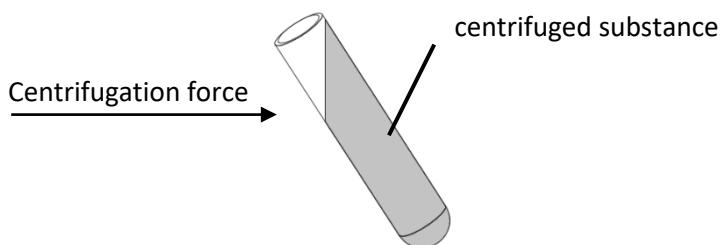

- | | |
|--|--|
| | <ul style="list-style-type: none"> If the manufacturer of the test tube has not specified the maximum level, fill the test tubes so that the centrifuged substance does not run out of the vessel during centrifugation. To do this, use the formula below: |
|--|--|


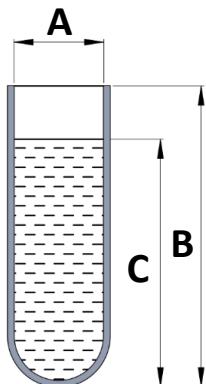


$$C < B - \frac{A}{2}$$

A – internal tube diameter
B – tube height
C – max liquid level

5.4 Filling the rotor

5.4.1 Angular rotors

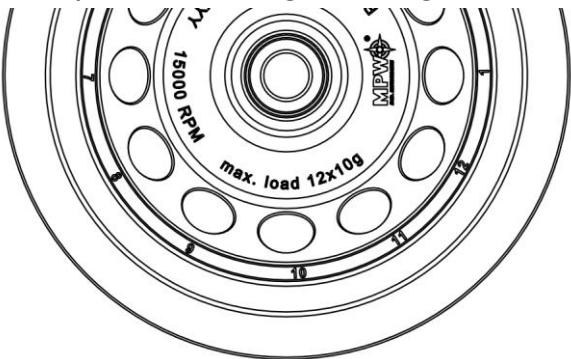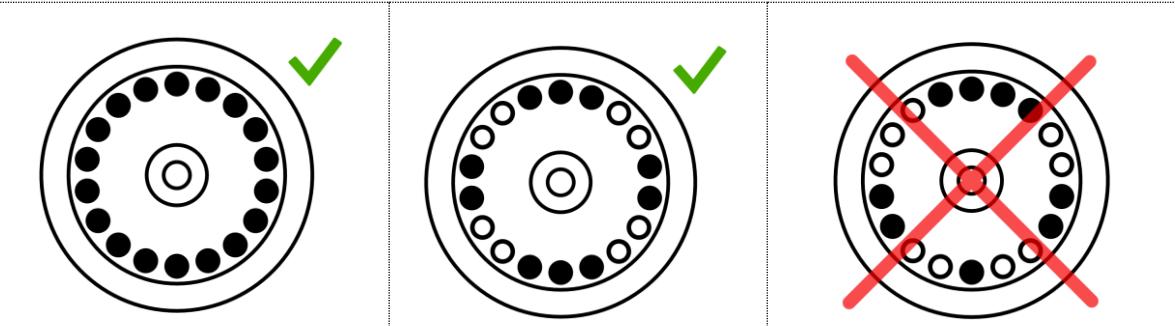	<p>CAUTION!</p> <ul style="list-style-type: none"> Angle rotors must be used with a suitable cover which must be screwed securely onto the rotor. The rotor and the cover are marked with the same catalog number (REF) to eliminate the risk of incorrect selection when you have several types of rotors.
	<p>An example of the marking on the angular rotor:</p>  <p>max. load 12x10g - means that 12 test tubes weighing 10 g each can be placed in the rotor.</p> <ul style="list-style-type: none"> To ensure symmetrical loading, insert test tubes of the same type and weight in pairs into opposite openings of the rotor. If reduction inserts are used, they should also be placed in the holes opposite to each other in pairs of the same type. <p>Examples of correct and incorrect arrangement of test tubes in the rotor:</p> 


5.4.2 Horizontal rotors

- Check that the impeller is seated correctly and firmly bolted to the motor shaft.
- Make sure that the rotor pins and grooves of the containers / hangers are clean, and then it is necessary to lubricate them with the technical petroleum jelly supplied with the device (catalog number 17201).
- Place the containers / hangers in the rotor.
- Horizontal rotors must be filled with a set of containers / hangers.
- Observe the limitations for the permissible centrifugal mass stated on the rotor and container. If the marking appears on the rotor, it refers to the mass of the substance to be centrifuged, and if on the container it refers to the mass of the contents of the container,

i.e. insert, test tube and the substance contained in it.

Examples of markings on containers for horizontal rotors:


Marking on the container

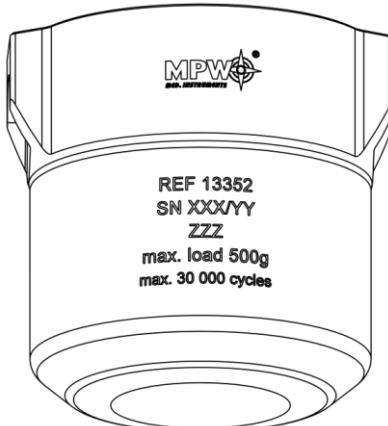

max. load 500g – maximum container load

- In order to ensure symmetrical and even rotor load, try to fill opposite seats with containers / hangers of the same type and weight.
- Tubes should be placed symmetrically facing each other.
- Before starting the centrifugation, check that all containers / hangers are properly placed in the rotor and can swing freely.
- For this purpose, empty test tubes should be placed in containers. Manually tilt the containers to the horizontal position and check that there are no collisions between the tubes, containers / hangers and the rotor.

Examples of correct and incorrect arrangement of test tubes in the rotor:

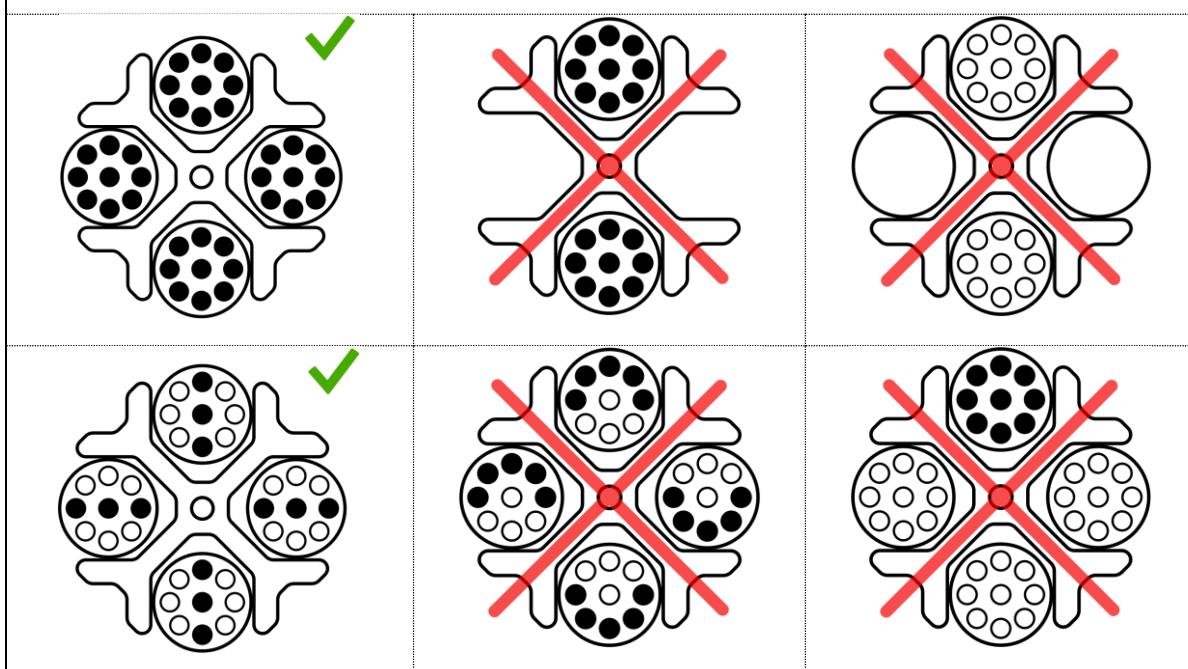

5.5 Safety hints



ROTOR MAINTENANCE

- In order to increase the durability of gaskets, threaded places, rotor pins, undercuts for pins in containers, they must be cleaned, and then it is necessary to

	<p>lubricate them with the technical petroleum jelly supplied with the device (catalog number 17201).</p> <p>The exception to this are the 12352 rotor pins, which are Teflon coated and do not require lubrication until the coating is worn out.</p> <ul style="list-style-type: none"> ▪ Use only accessories that are in good technical condition.
	<p>HU EQUIPMENT MAINTENANCE</p> <ul style="list-style-type: none"> ▪ Make sure the sealing rings (rubber) are lightly coated with grease to maintain tightness. Use high vacuum silicone grease, eg type "C" by LUBRINA.
	<p>HAZARDOUS MATERIALS</p> <ul style="list-style-type: none"> ▪ Infectious materials should be centrifuged only in containers / rotors with covers. ▪ It is not allowed to centrifuge toxic or infectious materials if the rotor or test tube seal is damaged. ▪ Appropriate disinfection procedures should always be carried out, if hazardous substances have contaminated the centrifuge or its accessories.
	<p>EXPLOSIVE, FLAMMABLE MATERIALS</p> <ul style="list-style-type: none"> ▪ It is not allowed to centrifuge explosive and inflammable materials. ▪ Do not centrifuge substances that could create a potentially explosive atmosphere as a result of the high energy supply during centrifugation. ▪ The centrifuge must not be used in an explosive atmosphere. ▪ It is not allowed to centrifuge materials that may generate flammable or explosive mixtures when exposed to air.

5.6 *Operating conditions*


	<p>GENERAL REMARKS</p> <ul style="list-style-type: none"> ▪ Only original equipment of centrifuges and spare parts should be used. ▪ In case of a malfunction of the centrifuge, the MPW MED factory service should be used. INSTRUMENTS or its authorized representatives. ▪ It is not allowed to start the centrifuge if it is not installed correctly or the rotor and accessories are not properly mounted. ▪ The centrifuge must not be transported with the rotor installed on the motor shaft. ▪ Fill the rotor equipment to the same weight in order to prevent unbalance of the centrifuge (point Filling the rotor).
---	---

	<p>START-UP</p> <ul style="list-style-type: none"> ▪ Before switching on the device, carefully read all sections of this manual in order to ensure the correct operation of the device and to avoid damage to the device or its accessories.
---	--

	<p>CENTRIFUGAL SUBSTANCES</p> <ul style="list-style-type: none"> ▪ Rotors are designed for centrifuging liquids with an average density of 1.2 g / cm³ or less. This applies to centrifugation at maximum speed. If liquids with a higher density are to be used, be sure to enter the density value in the PARAM / DENSITY tab in order to reduce the available spin speed.
---	--

5.7 Equipment life

- Each centrifugation cycle during which the rotor has been accelerated and decelerated is considered a work cycle, regardless of the speed and duration.
- Do not use rotors whose maximum number of cycles has already been exceeded or after the maximum service life of the centrifuge has elapsed (the service life of the device is 10 years from the date of purchase of the device), depending on which comes first.
- The number of permissible and completed cycles for a given rotor can be found in the centrifuge menu - Menu/Rotor cycles (description in the chapter Rotor cycles). The centrifuge log records data on the types of rotors used.
- The user should record the work cycles for rotors and containers using their own method. The centrifuge does not recognize changes or replacements of rotors or containers of the same type.
- Below is an example of the marking on the rotor and container:

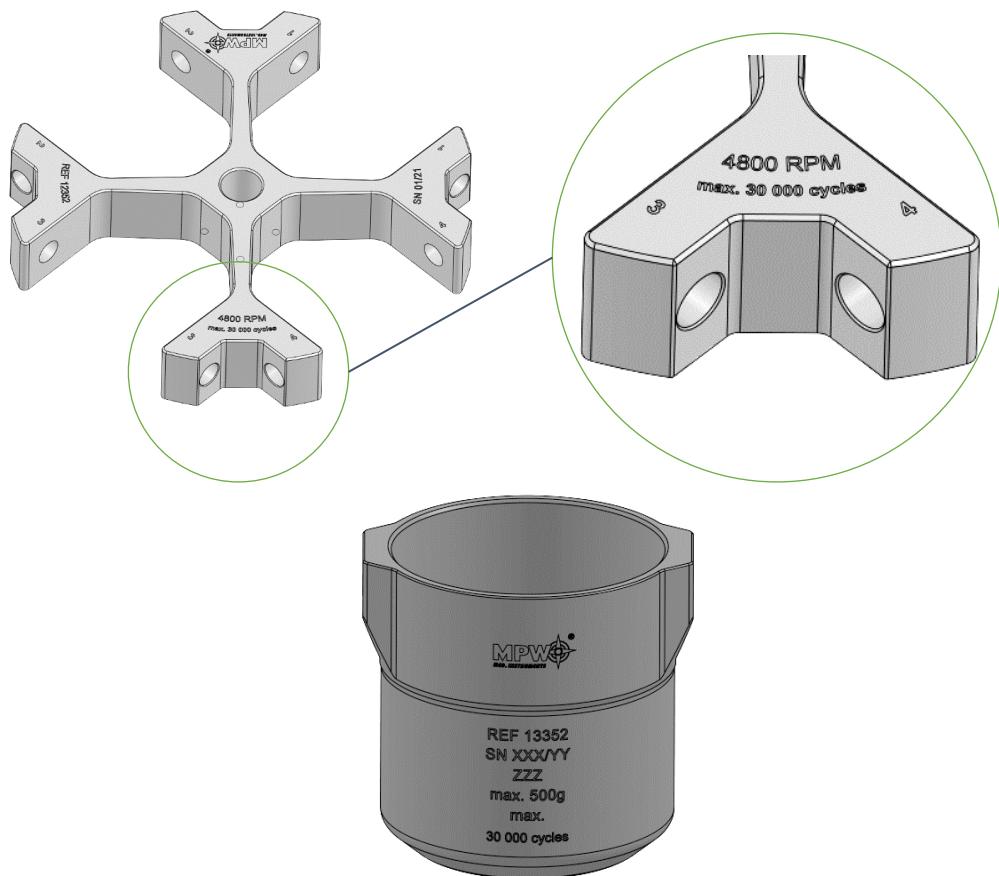

Type of equipment	Allowed number of cycles	Permitted work period
Rotor 12352	30000	5 years
Rotors from the list (see Attachments)	15000	10 years of centrifuge operation

5.8 Service life of rubber suspension components of the drive unit

The shelf life of the rubber suspension components of the drive unit is **3 years** (counted from the date of purchase). After this time, they must be replaced with new ones.

5.9 Work safety

The centrifuge should be inspected by an authorized service at least once a year (after the warranty period). The reason for more frequent inspections may be special circumstances, e.g. a corrosive environment. The tests should end with the issuance of a validation protocol specifying the verification of the technical condition of the laboratory centrifuge.

The centrifuge is accompanied by a **technical passport**, in which entries should be made from the performed service activities such as: repairs, technical inspections, and replacement of components and equipment with a specified durability date (suspension, rotors, containers). Exceeding the service life of components with a specified durability date (suspension, rotors, containers) will result in a negative assessment of the centrifuge during annual inspections.

	CONTROLS CONDUCTED BY THE OPERATOR <ul style="list-style-type: none">▪ Centrifuge accessories, especially structural changes, corrosion, initial cracks, abrasion of metal parts.▪ Bolted connections.▪ Inspection of rotor and container seals, if any. Particular attention should be paid to rubber elements (seals). In the event of any damage or visible structural changes, they should be immediately replaced with new ones.▪ Control of the performance of annual post-warranty inspections of the technical condition of the centrifuge.▪ During centrifugation, it is not allowed to lift, shift the centrifuge or rest on it.▪ During centrifugation one must not stay in the safety zone, i.e., 30 cm distance around the centrifuge, nor leave any objects, e.g., glass vessels, inside this zone.▪ It is not allowed to put any objects on the centrifuge.
	OPENING THE COVER DURING SPINNING <ul style="list-style-type: none">▪ It is not allowed to use the emergency cover opening during centrifuging, because it may result in loss of health or life.
	HANDLING OF ROTORS <ul style="list-style-type: none">▪ It is not allowed to use accessories (rotors, lids, containers, hangers and round carriers) with signs of corrosion or other mechanical damage.▪ It is not allowed to centrifuge substances of high corrosive aggressiveness, which may damage the materials and reduce the mechanical properties of rotors, buckets and round carriers.▪ It is not allowed to centrifuge rotors with removed or loose covers.

5.10 Unbalance



Unbalance causes noise, vibration during operation and has a negative effect on the driveline (engine and suspension). The more precisely the process of balancing the feed to the rotor is carried out, the smoother the centrifuge will run and the longer the useful life of the drive system will be. Moreover, thanks to the correct balancing, an excellent level of separation of the centrifuged substance is achieved since the separated components will not be picked up again by vibrations.

The centrifuge is equipped with a rotor imbalance sensor. In the event of its activation, the centrifugation process is stopped by quick braking and an error message is displayed. Erasing the error message is possible by pressing one of the following buttons: **BACK**, **STOP**, **COVER**, **SET** and **▲ ▼ ◀▶**.

Make sure that the rotor has been properly loaded - places in the rotor must be equipped with identically filled containers, inserts and test tubes so as to obtain the best possible weight balance (see chapter Filling the rotor). If necessary, correct the load distribution and / or, in the case of horizontal rotors, clean and lubricate the rotor pins, then restart the spin.

5.11 Emergency stop

At any time during centrifugation, it is possible to interrupt the process and stop the centrifugation with the fastest rotor characteristics. This is done by pressing the stop button twice (**2x STOP**).

Pressing the **STOP** key once will stop the spinning with the braking characteristics set in the program. The message about interrupted centrifuging can be canceled with the following buttons: **BACK**, **STOP**, **COVER**, **SET** and **▲ ▼ ◀▶**.

5.12 Residual risk

The centrifuge is built according to the state-of-the-art and the recognized safety regulations. Nevertheless, still remain some level of residual risk due to improper operation and malfunctions. It is possible to decrease residual risk by strictly applying user manual conditions and correcting malfunction which could threaten safety, immediately.

5.13 Obligation to report a serious device incident


Any serious incident related to the device should be reported to the manufacturer and the competent authority of the Member State where the user or patient resides.

6 Product description

6.1 Product Design and Appearance


A new generation of MPW MED laboratory centrifuges. INSTRUMENTS is equipped with modern microprocessor controllers, very durable and quiet brushless asynchronous motors and equipment that meets modern user requirements.

The centrifuge has a rigid self-supporting structure. The housing is made of aluminum sheet, the back is made of steel sheet, and the rotating chamber is made of stainless steel. The front part and cover are made of ABS plastic. The cover is mounted on steel hinge axles, and from the front it is secured against opening during spinning with an electromagnetic lock.

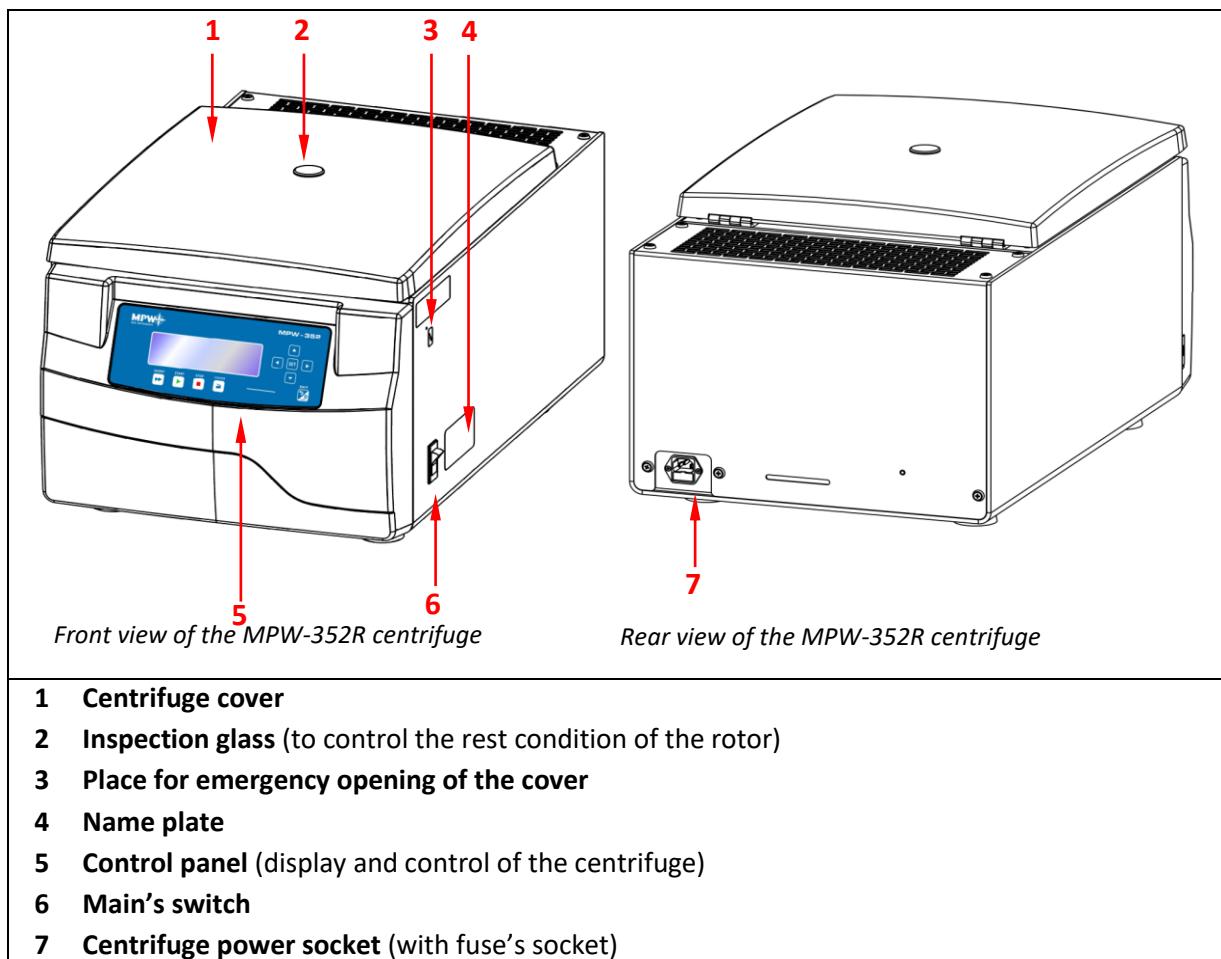

6.2 Name plate

Data regarding the device should be read from the nameplate located on the side wall of the centrifuge next to the power switch (the image below is an example).

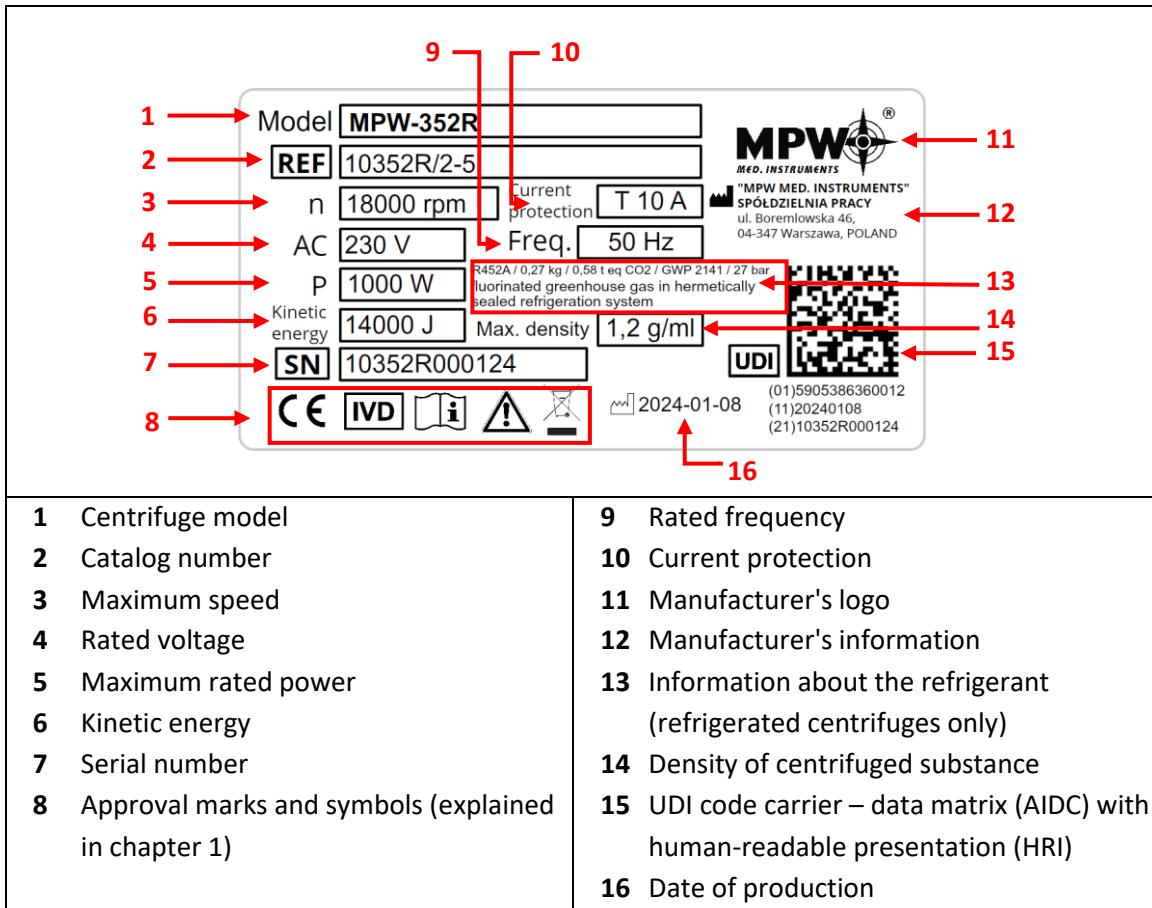

6.3 Control device

The microprocessor control unit of the centrifuge ensures broad possibilities of providing, realization and reading of work parameters.

6.4 Setting parameters

Data setting and read-out system forms hermetically closed keyboard with distinctly accessible operation points. Easily readable displays signaling individual performed operations facilitate operator's programming and recording of parameters and condition of the centrifuge.

6.5 Safety features

Cover lock

The centrifuge can be started only with properly closed cover. While the cover can be opened only after stopping the rotor. In case of emergency opening of the cover during operation, the centrifuge drive will be immediately switched-off and the rotor will brake till complete stopping.

Unbalance detecting

When loads of opposite buckets or carriers in rotors are unbalanced, the drive will be switched-off during acceleration or operation of the centrifuge – and the error message will be displayed.

Rotor verification and checking compatibility with loaded program

Directly after starting centrifuging, a unit verifies the type of the rotor applied and in the case of its incompatibility with the type indicated in the application or absence of the rotor, the spinning process shall be stopped with simultaneous displaying the error message. The conformity of the type of the rotor is

signaled with a single audible signal. In case autoidentification (see 9.8 Other) option is checked, proper rotor will be automatically chosen, without user engagement.

Rest state inspection

Opening the centrifuge lid with the **COVER** key is possible only when the rotor is at rest. Check that the symbol  described in the **Display** chapter is visible on the screen. Use the sight glass on the cover to make sure the impeller is not turning. When the rotor brakes, the symbol  described in the **Display** section is visible. Emergency opening of the cover during rotor spinning is not allowed.

Checking of excessive temperature

If temperature in rotation chamber exceeds 50°C (MPW-352) / 65°C (MPW-352R/RH) caused by, for example, malfunction of cooling system, drive will be switched off and error message will be displayed. The reboot is only possible after chilling device.

6.6 Increase in temperature (MPW-352 only)


In uncooled centrifuges, the temperature in the rotor chamber, rotor and sample can increase to above 40°C, based on the run time, g-force (RCF)/speed and ambient temperature.

7 Centrifuging

Power switching ON/OFF is carried out with master switch situated on the right-side wall of the centrifuge. All settings on the centrifuge are done by means of the control panel.

7.1 Control panel

The control panel placed on the front casing serves the purpose of controlling centrifuge operation.

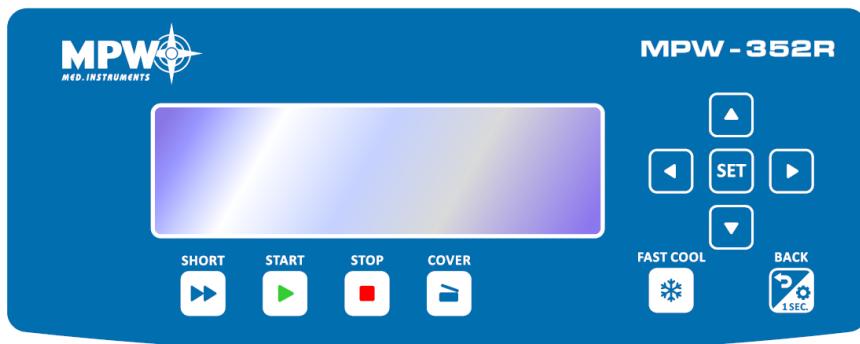

Control panel

▶▶	SHORT ¹	short-time centrifuging
▶	START	start centrifugation run
■	STOP ²	end centrifugation run
◀	COVER	cover opening
❄	FAST COOL	start fast cooling mode (MPW-352R and MPW-352RH only)
◀ 1SEC	BACK/ OPTIONS	exit the current menu / enter to submenu of options (keep held down within 1 s.)
▲	UP	navigation in menu / increasing values
▼	DOWN	navigation in menu / decreasing values
◀	LEFT	navigation in menu
▶	RIGHT	navigation in menu
SET	SET	changing parameters / confirming changes

¹ the centrifuge is working as long as the key is pressed

² first press - spin stop with the currently selected braking characteristic (then confirm the message with the SET or STOP button),
second press - the fastest possible stop.

7.2 Display

The display is located in the center of the control panel. The main screen variants are presented below. In the user manual exemplary screens from MPW-352R/352RH are shown. For MPW-352 (without refrigeration) temperature is not shown. Blinking of field on display mean it is ready to set. Blinking of field is visualized as highlighted in the user manual.

	After switching on centrifuge, welcome screen appears. After disappearing the welcome screen, it is possible to setting up parameters.
--	--

	Simplified display mode is set as default, there is possible to switch to normal (see chapter "Types of main screen").
	Normal display contains an expanded number of settings visible during operation.

Detailed information on display modes is provided in chapter **Types of main screen**.

SPEED	rotor speed	assigned/measured
RCF	relative centrifugal force	assigned/measured
TIME	centrifuging time	assigned/measured
TEMP	temperature	assigned/measured
PRG	program no.	
11199	rotor no.	
PARAM	parameters of the centrifuge	
MENU	configuration menu	

	changing values		
	user multi sections curve		
	density > 1,2 g/cm ³		
	centrifuging radius changed		
	counting time down (decreasing)		counting time up (increasing)
	cooling to assigned temperature		
	FAST COOL mode cooling		
	centrifuging		centrifuging (with automatic cover opening)
	rotor stopped / closed cover		rotor stopped / opened lid
	braking		fastest decelerating
	rotor identification		
	thermal chamber		
	temperature delay		
	time delay		
	drop-down list		
	temporarily disabled		
	locked		
	time counting (blinking)		
	disabled option		active option

7.3 Setting up RPM, RCF, time, temperature

On the main screen, it is possible to set:

rotating speed - RPM	SPEED
relative centrifugal force (multiple of g-force)	RCF
centrifuging time	TIME
centrifuging temperature	TEMP (R/RH only)


Exemplary change of **SPEED** setting:

	<ul style="list-style-type: none"> Press SET (to enter edit mode) –  appears. Via ▲▼◀▶ keys mark SPEED field (blinking). Press SET  blinking. Via ◀▶ choose order of magnitude of changing value (blinking). With ▲▼ choose demanded value. Repeat above two steps for other orders of magnitude. Confirm settings by pressing SET. Exit edit mode by pressing BACK.
When RPM is changed, RCF is automatically corrected.	

Exemplary change of **RCF** setting:

	<ul style="list-style-type: none"> Press SET (to enter edit mode) –  appears. Via ▲▼◀▶ keys mark RCF field (blinking). Press SET  blinking. Via ◀▶ choose order of magnitude of changing value (blinking). With ▲▼ choose demanded value. Repeat above two steps for other orders of magnitude. Confirm settings by pressing SET. Exit edit mode by pressing BACK.
When RCF is changed, RPM is automatically corrected.	

Exemplary change of **TIME** setting:

	<ul style="list-style-type: none"> Press SET (to enter edit mode) –  appears. Via ▲▼◀▶ keys mark TIME field (blinking).
	<ul style="list-style-type: none"> Press SET  blinking. Via ◀▶ choose order of magnitude of changing value (blinking).

e.g.: centrifuging time – 2 minutes 00 seconds	<ul style="list-style-type: none"> With ▲▼ choose demanded value. Repeat above two steps for other orders of magnitude. Confirm settings by pressing SET. Exit edit mode by pressing BACK.
00:02:00	set value
02:00	current value (most significant digits)

HOLD mode	continuous run mode
	<ul style="list-style-type: none"> To run centrifuging in HOLD mode set 00:00:00 time. To end centrifuging in HOLD mode press STOP.

Exemplary change of TEMP setting:	
	<ul style="list-style-type: none"> Press SET (to enter edit mode) – appears. Via ▲▼◀▶ keys mark TEMP field (blinking). Press SET key. With ▲▼ choose demanded value [-20°C÷40°C]. Confirm settings by pressing SET. Exit edit mode by pressing BACK.


7.4 Users programs

	After switching centrifuge on, program that was used in previous session is being loaded. If any program was not used in previous session, centrifuge resume the last chosen parameters.
--	--

Program choosing:	
-------------------	--

Entering the program selection mode for the simplified display :	
---	--


	<ul style="list-style-type: none"> Press and hold by 1 second. Choose PROG with ▲▼ Press SET.
Entering the program selection mode for the normal display :	

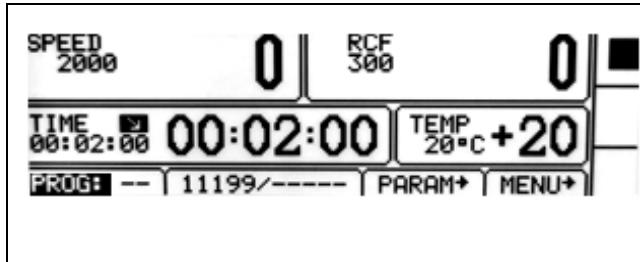

- Press **SET** key – appears.
- Via **▲▼◀▶** keys mark **PRG-** – field (begin blinking)
- Press **SET** key – list of programs is visible.

Program selection mode tab:									
No SPEED RCF TIME TEMP ACC DEC ROT									
0 4590 2826 HOLD 20 0 0 11740									
1 4590 2826 00:01:00 20 0 0 11740									
► 2 5090 3476 00:02:00 20 0 0 11740									
3 4 5									
No SPEED					C DEC ROT				
0 4590 LOAD 0 0 11740									
1 4590 SAVE 0 0 11740									
► 2 5090 DELETE 0 0 11740									
3 CURVES 4 5									
No SPEED					C DEC ROT				
0 4590 NEW PROGRAM									
1 2 3 4 5									
No SPEED					C DEC ROT				
0 4590 1 4590 ► 2 5090									
3 4 5									
No SPEED					C DEC ROT				
0 4590 1 4590 ► 2 5090									
3 4 5									
No SPEED					C DEC ROT				
0 4590 1 4590 ► 2 5090									
3 4 5									

Creating a new program:

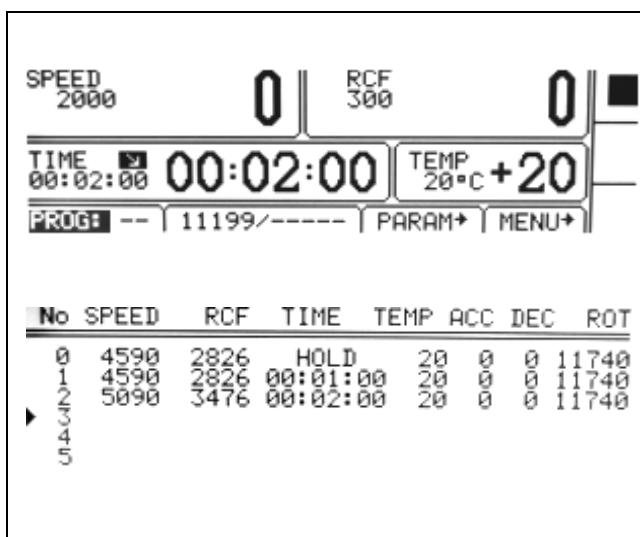

- Press **SET** key.
- Via **▲▼◀▶** keys mark **PROG** field (blinking).
- Press **SET** key. List of programs is visible, choose demanded position (number of program).
- Press **SET** key- menu of program settings will appear.
- Choose **NEW PROGRAM** press **SET** and **BACK**, and then set demanded parameters of centrifuging (look chapter **Centrifuging**).
- In case you want to register new program, back to the **PROG** menu and

No SPEED	LOAD SAVE DELETE CURVES NEW PROGRAM	C DEC ROT	save it as described before.
----------	---	-----------	------------------------------

▪ Changing parameters during centrifuging




There is a possibility to change parameters: **SPEED**, **RCF**, **TIME**, **TEMP** during centrifuging.

Such modifications inactivate currently running program. When program was set, modification during run is represented by **PROG --** symbol (instead of the program number).


7.5 Creator of acceleration and deceleration curves

PROG/CURVES							
No SPEED	RCF	TIME	TEMP	ACC	DEC	ROT	
0 4590	2826	HOLD		20	0	0	11740
1 4590	2826	00:01:00		20	0	0	11740
► 2 5090	3476	00:02:00		20	0	0	11740
3							
4							
5							
No SPEED	LOAD SAVE DELETE CURVES NEW PROGRAM	C DEC ROT					
0 4590		0 0 11740					
1 4590		0 0 11740					
► 2 5090		0 0 11740					
3							
4							
5							
No SPEED	PROGRAM: 2 CURVES	C DEC ROT					
0 4590		0 0 11740					
1 4590		0 0 11740					
► 2 5090	ACCELERATION DECELERATION	0 0 11740					
3							
4							
5							

7.5.1 Acceleration characteristic, creation of episode 1

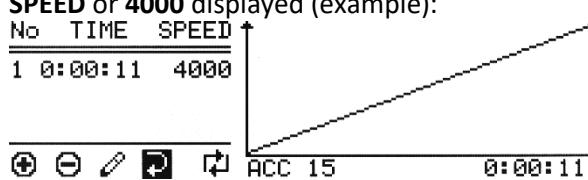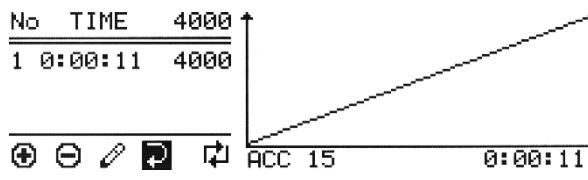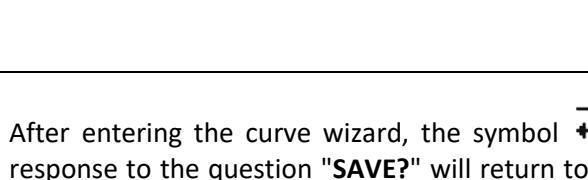
SPEED or 4000 displayed (example):  <table border="1"> <tr> <td>No</td> <td>TIME</td> <td>SPEED</td> </tr> <tr> <td>1</td> <td>0:00:11</td> <td>4000</td> </tr> </table>  <table border="1"> <tr> <td>No</td> <td>TIME</td> <td></td> </tr> <tr> <td>1</td> <td>0:00:11</td> <td>4000</td> </tr> </table>  <table border="1"> <tr> <td>No</td> <td>TIME</td> <td></td> </tr> <tr> <td>1</td> <td>0:00:11</td> <td>4000</td> </tr> </table> 	No	TIME	SPEED	1	0:00:11	4000	No	TIME		1	0:00:11	4000	No	TIME		1	0:00:11	4000	No	section no. (max. 4)
No	TIME	SPEED																		
1	0:00:11	4000																		
No	TIME																			
1	0:00:11	4000																		
No	TIME																			
1	0:00:11	4000																		
TIME	total acceleration time																			
SPEED	final RPM																			
ACC	characteristic's no. (10-19)																			
+	adding a new section																			
-	deleting last section																			
✎	editing sections																			
➡	exiting from characteristics wizard																			
↔	switching RPM/RCF																			

After entering the curve wizard, the symbol  is highlighted. Pressing **SET** and selecting "NO" in response to the question "SAVE?" will return to the **PROG → CURVES** menu without making changes to the starting characteristics. To start editing the one-segment characteristics, select the icon  with the **◀▶** keys and press the **SET** key.

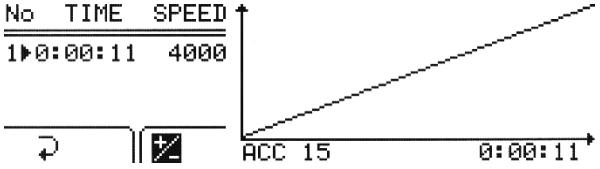
		editing value (flashing means editing the given value)
No TIME SPEED 1 0:00:11 4000 		<ul style="list-style-type: none"> ▪ Press SET ▪ With ▲▼◀▶ choose time for section ▪ Press SET ▪ It is not possible to edit the maximum speed value. To do this, more sections have to be created, but the last section will always have the maximum set speed and cannot be changed. ▪ Select  with ▼◀ buttons and press SET to finish editing characteristics.

7.5.2 Adding and editing sections - acceleration

To program next sections, select the  icon with the ◀▶ buttons and press SET . A new section (sections) will appear with a time of 1 second and a speed equal to the maximum speed. To start editing a newly added section (sections), select the  icon with the ◀▶ buttons and press SET , and follow the instructions given below. After entering the profile section editing menu, the time value of the first section will be highlighted (see the picture below).
--

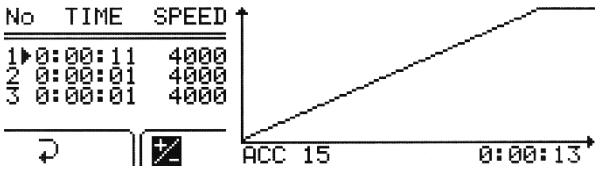
No TIME SPEED 1 0:00:11 4000 2 0:00:01 4000 3 0:00:01 4000 	The maximum speed value for the section cannot be higher than the maximum speed value for the characteristic (for the last section).
	<ul style="list-style-type: none"> ▪ With ▲▼◀▶ highlight time or speed for desired section ▪ Press SET ▪ With ▲▼◀▶ choose value ▪ Press SET ▪ Repeat until setting all the sections ▪ To finish editing characteristic with ▲▼◀▶ choose  and press SET. Finishing edition can be also done by pressing BACK button

Saving created characteristic

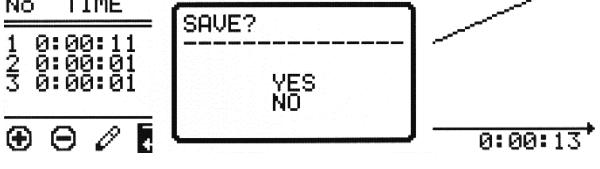No TIME 1 0:00:11 2 0:00:01 3 0:00:01 	<ul style="list-style-type: none"> ▪ Select the  icon with the ◀▶ buttons and press SET ▪ In the "Save?" window, use ▲▼ buttons to select YES to confirm saving the characteristic or NO, to exit without saving ▪ Press SET
---	---


7.5.3 Acceleration graph

An example of given parameters and a graph:

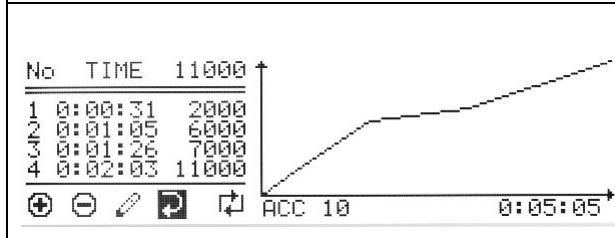


After programming the time and / or speed values, the segment (all segments) is graphically displayed on the graph on the right side of the screen. The time value is on the horizontal axis of the user's starting characteristic, while the speed is on the vertical axis.

7.5.4 Deceleration characteristic – creating section 1

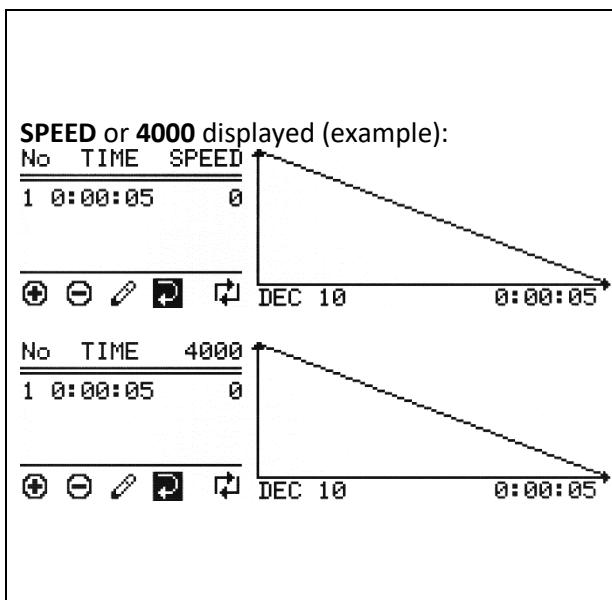

NO	section no. (max. 4)
TIME	total acceleration time
SPEED	final RPM
DEC	characteristic's no. (10-19)
	adding a new section
	deleting last section
	editing sections
	exiting from characteristics menu
	switching RPM/RCF

After entering the curve wizard, the symbol is highlighted. Pressing **SET** and selecting "NO" in response to the question "**SAVE?**" will return to the **PROG → CURVES** menu without making changes to the starting characteristics. To start editing the one-segment characteristics, select the icon with the **◀▶** keys and press the **SET** key.

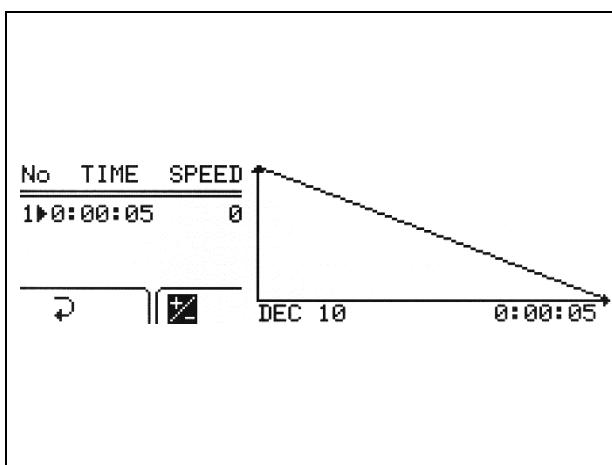

	editing value (flashing means editing the given value)
<ul style="list-style-type: none"> ▪ Press SET ▪ With ▲▼◀▶ choose time for section ▪ Press SET ▪ To edit speed ▪ It is not possible to edit the minimum speed value. To do this, more legends must be created, but the last leg will always be "0". ▪ Select with ▼◀ buttons and press SET to finish editing characteristics 	


7.5.5 Adding and editing sections - deceleration

In order to program successive periods, select the icon with the **◀▶** keys and press the **SET** key. A new segment (or segments - after successive presses of SET) will appear with the time and speed equal to the minimum speed - "0".

To start editing the newly added sections, select the icon with the **◀▶** buttons, press **SET** and make

the settings as described below.


After entering the profile section editing menu, the time value of the first section will be highlighted (see the picture below).

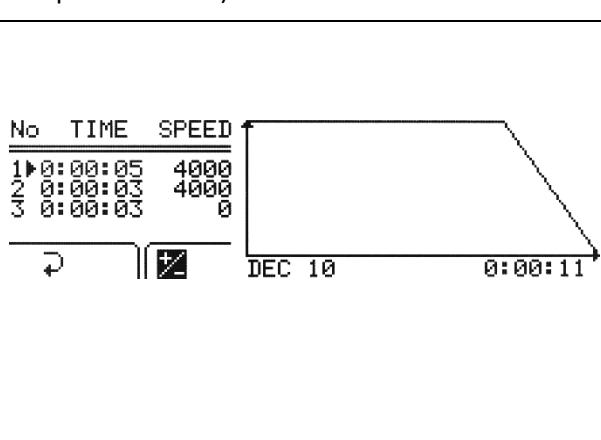

The speed value of the last segment will always be "0"

- With **▲▼◀▶** highlight time or speed for desired section
- Press **SET**
- With **▲▼◀▶** choose value
- Press **SET**
- Repeat until setting all the sections
- To finish editing characteristic with **▲▼◀▶** choose and press **SET**. Finishing edition can be also done by pressing **BACK** button


Saving created characteristic

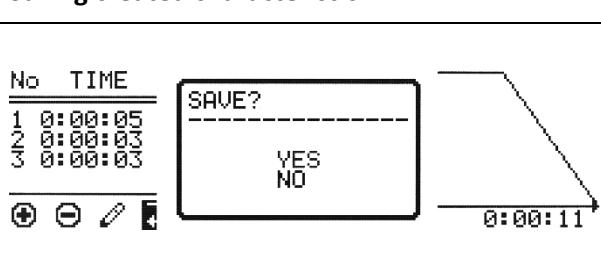

- Select the icon with the **◀▶** buttons and press **SET**
- In the "Save?" window, use **▲▼** buttons to select YES to confirm saving the characteristic or NO, to exit without saving
- Press **SET**

7.5.6 Deceleration graph


An example of given parameters and a graph:

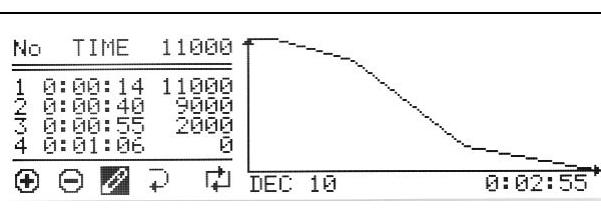

After programming the time and / or speed values, the segment (all segments) is graphically displayed on the graph on the right side of the screen. The time value is on the horizontal axis of the user's braking characteristic, while the speed is on the vertical axis.

7.5.7 Deleting sections

In the characteristic's wizard:

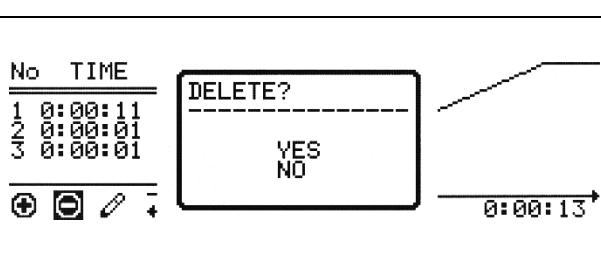

- Select the icon with the **◀▶** buttons and press **SET**
- In the "Delete?" window, use **▲▼** buttons to select YES to confirm deleting the characteristic section or NO to cancel
- Press **SET**

7.6 Programs with user characteristics

Loading a modified program in the CURVES fold is signaled by the icon on the main screen:



Icon signals that program with user acceleration/deceleration characteristics are loaded.

A change in any parameter entails the deactivation of the multi-section's curves mode.

7.7 Rotor choosing


Simplified display mode	<ul style="list-style-type: none"> Press and hold BACK by 1 second. Choose rotor number (exemplary 11199/----) with ▲▼. Press SET. Execute points described follow (below Normal display mode description) 																																																	
	Normal display mode <ul style="list-style-type: none"> Press SET appears – Via ▲▼◀▶ mark rotor choosing field. Press SET (Rotor list will appear). <table border="1"> <thead> <tr> <th>NO</th> <th>ROTOR</th> <th>BUCKET</th> <th>SPEED</th> <th>RCF</th> <th>RMAX</th> <th>RMIN</th> </tr> </thead> <tbody> <tr> <td>1</td> <td>11199</td> <td>-----</td> <td>18000</td> <td>24270</td> <td>67</td> <td>35</td> </tr> <tr> <td>2</td> <td>11210</td> <td>-----</td> <td>5000</td> <td>3997</td> <td>143</td> <td>60</td> </tr> <tr> <td>3</td> <td>11211</td> <td>-----</td> <td>5500</td> <td>4498</td> <td>133</td> <td>87</td> </tr> <tr> <td>4</td> <td>11213</td> <td>-----</td> <td>5500</td> <td>4227</td> <td>125</td> <td>79</td> </tr> <tr> <td>5</td> <td>11259</td> <td>-----</td> <td>15000</td> <td>24400</td> <td>97</td> <td>65</td> </tr> <tr> <td>6</td> <td>11273</td> <td>-----</td> <td>12000</td> <td>14006</td> <td>87</td> <td>54</td> </tr> </tbody> </table> <ul style="list-style-type: none"> It is possible to set AUTOMATIC ROTOR IDENTIFICATION. The procedure is described in subsection OTHERS 	NO	ROTOR	BUCKET	SPEED	RCF	RMAX	RMIN	1	11199	-----	18000	24270	67	35	2	11210	-----	5000	3997	143	60	3	11211	-----	5500	4498	133	87	4	11213	-----	5500	4227	125	79	5	11259	-----	15000	24400	97	65	6	11273	-----	12000	14006	87	54
NO	ROTOR	BUCKET	SPEED	RCF	RMAX	RMIN																																												
1	11199	-----	18000	24270	67	35																																												
2	11210	-----	5000	3997	143	60																																												
3	11211	-----	5500	4498	133	87																																												
4	11213	-----	5500	4227	125	79																																												
5	11259	-----	15000	24400	97	65																																												
6	11273	-----	12000	14006	87	54																																												

7.8 SHORT mode

	<ul style="list-style-type: none"> The SHORT mode is activated by pressing and holding ►(SHORT). In SHORT mode the centrifuge is working as long as the SHORT key is pressed or when set time is over. The spin cycle is finished when the SHORT button is released.
--	--

7.9 Finishing the centrifuging

	When preselected time is reached, centrifugation will end automatically.
	Before lapsing preselected time, one may stop centrifuging. Pressing STOP for the first time will stop centrifuging with the characteristic set-in loaded program.
	Pressing STOP second time will stop centrifuging with the fastest characteristic.

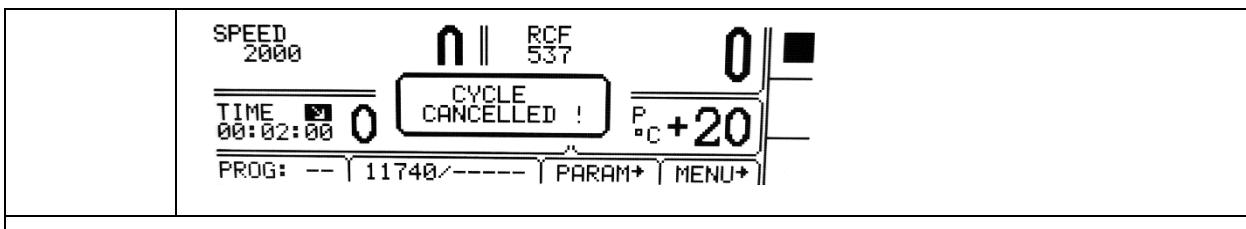

The message about cancel of centrifuging can be delete with the **STOP**, **SET**, **COVER**, **▲▼◀▶** or **BACK** key.

7.10 Temporarily disabled functions

Functions written below can be temporarily disabled.

active	SPEED	RCF	TIME	TEMP	PROG —	— / —	PARAM	MENU
THERMAL CHAMBER	•	•	•	○	•	•	•	•
STANDARD CENTRIFUGING	•	•	•	•	•	○	•	○

• available

○ disabled



8 Temperature control



MPW-352R and MPW-352RH only

Centrifuge is equipped with ecological refrigerating system with temperature control. During centrifugation, there may appear differences in temperature on the display and temperature of the samples in the rotor. It depends on thermal conductivity of the rotor, and samples and centrifugation time, initial temperature of rotor and samples.

Exemplary change of **TEMP** setting:

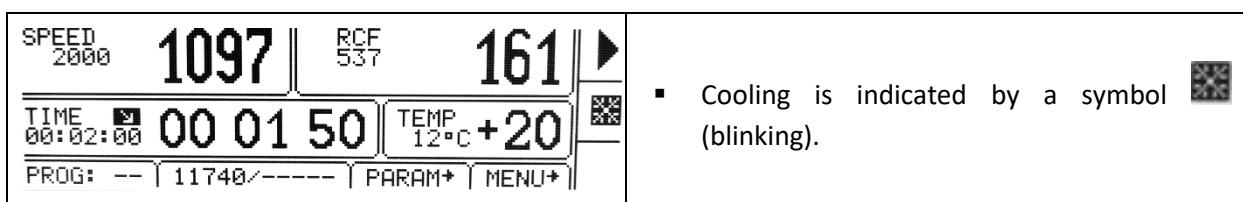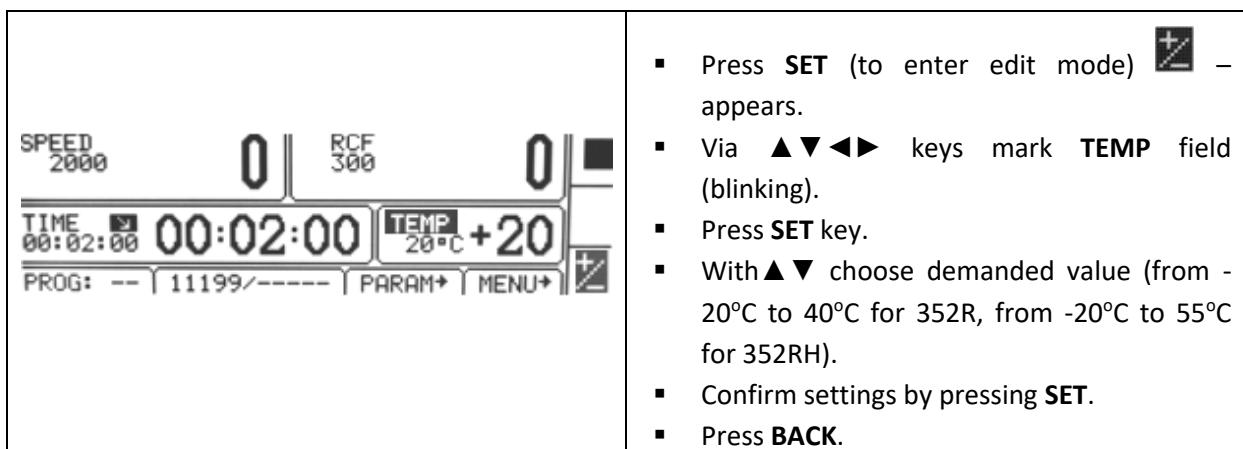

8.1 Initial cooling during centrifuging –FAST COOL

	The parameters allowable to change at FAST COOL mode: <ul style="list-style-type: none"> temperature (lower than current temperature shown by centrifuge)
--	---

	<ul style="list-style-type: none"> In order to centrifuging reduced temperature samples (e.g., storage in the external refrigerator) centrifuge chamber, rotor and centrifuge container must be pre-cooling to the predetermined temperature. It causes minimalization of temperature differences. Initial cooling may be activated by FAST COOL key (lid must be closed – rotor is spinning at FAST COOL mode) When FAST COOL mode is active, cooling system automatically set proper parameters to obtain demanded temperature the fastest way.
--	---



FAST COOL mode is marked by symbol XX XX blinking in the right upper side of display.



It is possible to exit **FAST COOL** mode at any time by pressing **STOP** key.
 Interruption of the function is signaled by a message.

8.2 Initial cooling or heating without centrifuging – THERMAL CHAMBER

	PARAM → THERMAL CHAMBER
	<ul style="list-style-type: none"> There is possible to run centrifuge in THERMAL CHAMBER mode - cooling for R, cooling and heating for RH (rotor is at standstill). How to enable THERMAL CHAMBER is described in Parameters of centrifugation chapter.

8.3 Cooling or heating in “START DELAY – OF TEMPERATURE” mode

	PARAM → START DELAY – OF TEMPERATURE
	<ul style="list-style-type: none"> Centrifuging process will start, when preselected temperature is reached. How to enable run START DELAY – OF TEMPERATURE function is described in Parameters of centrifugation chapter.


8.4 Cooling or heating in „SHORT” mode

	<ul style="list-style-type: none"> Cooling and heating features are available in SHORT mode. How to enable run centrifugation in SHORT mode is described in Centrifugation/SHORT mode.

8.5 Cooling and heating notes

Centrifuges with cooling (MPW-352R and MPW-352RH) are equipped with an efficient cooling system. It allows obtaining selected temperatures in the chamber even at maximum spin speed or fast obtaining desired temperatures (e.g., 4°C and 36°C). Note that time and possibility of obtaining a set temperature is dependent on multiple factors, including: the power of the cooling system, the shape of the rotor, the rotor speed, ambient temperature, etc. The accuracy of the temperature stability of ± 1 ° C (for 352R), ± 3 ° C (for 352RH) is determined by the installation place of the temperature sensor.

9 Parameters of centrifugation

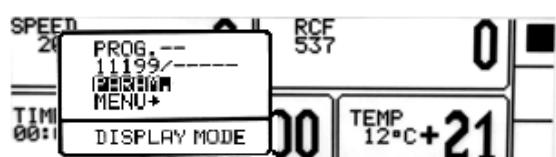
Simplified display	 <ul style="list-style-type: none"> Press and hold  by 1 second. Choose PARAM. with  Press SET. Execute points described follow (below Normal display mode description)
Normal display	 <ul style="list-style-type: none"> Press SET. With  keys select PARAM. Press SET.
PARAMETERS	<p>ACCELERATION 3 <input type="checkbox"/> THERM. CHAMB. DECELERATION 3 <input type="checkbox"/> AUTOM. LID OPENING RADIUS (mm) 120 <input type="checkbox"/> START DELAY DENSITY (g/cm³) 1.5 TEMP. OFFSET(°C) 0 CHAMBER DEL.(min) 1</p>

ACCELERATION	chosen acc. characteristic (0-the fastest, 9-the slowest)
DECELERATION	chosen dec. characteristic (0-the fastest, 9-the slowest)
RADIUS [mm]	current rotor radius [mm]
DENSITY (g/cm³)	sample density [g/cm³]
TEMP. OFFSET (°C)	value of temperature correction
CHAMBER DEL. (min)	delay between set thermal chamber mode and start it
THERMAL CHAMBER	cooling of the chamber without centrifuging
AUTOM. LID OPENING	opening cover after centrifuging automatically
START DELAY	starting delayed (after pressing START)


9.1 Acceleration/deceleration – changing characteristics

PARAMETERS	<ul style="list-style-type: none"> With  select ACCELERATION or DECELERATION. Press SET. With  select demanded number of characteristics. Press SET. ACCELERATION – 10 (0 ÷ 9), linear accelerating characteristics assigned to every rotor. 0-the fastest acceleration, 9-the slowest acceleration. DECELERATION – 10 (0 ÷ 9), linear decelerating characteristics assigned to every rotor. 0-the fastest deceleration, 9-the slowest deceleration.
ACCELERATION 3 <input type="checkbox"/> THERM. CHAMB. DECELERATION 3 <input type="checkbox"/> AUTOM. LID OPENING RADIUS (mm) 120 <input type="checkbox"/> START DELAY DENSITY (g/cm³) 1.5 TEMP. OFFSET(°C) 0 CHAMBER DEL.(min) 1	

9.2 Radius
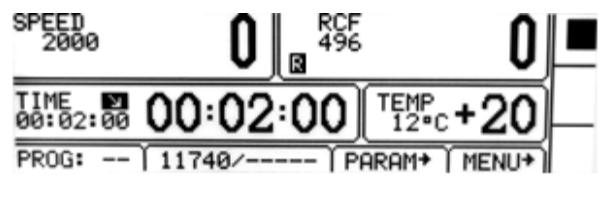
<p>PARAMETERS</p> <table border="0"> <tr> <td>ACCELERATION</td> <td>3</td> <td><input type="checkbox"/> THERM.CHAMB.</td> </tr> <tr> <td>DECELERATION</td> <td>3</td> <td><input type="checkbox"/> AUTOM.LID OPENING</td> </tr> <tr> <td>RADIUS (mm)</td> <td>120</td> <td><input type="checkbox"/> START DELAY</td> </tr> <tr> <td>DENSITY (g/cm³)</td> <td>1.5</td> <td></td> </tr> <tr> <td>TEMP.OFFSET(°C)</td> <td>0</td> <td></td> </tr> <tr> <td>CHAMBER DEL.(min)</td> <td>1</td> <td></td> </tr> </table>	ACCELERATION	3	<input type="checkbox"/> THERM.CHAMB.	DECELERATION	3	<input type="checkbox"/> AUTOM.LID OPENING	RADIUS (mm)	120	<input type="checkbox"/> START DELAY	DENSITY (g/cm³)	1.5		TEMP.OFFSET(°C)	0		CHAMBER DEL.(min)	1		<ul style="list-style-type: none"> ▪ RADIUS [mm] - control of the radius of the rotor within the range from R_{\min} to R_{\max}. Available values depend on chosen rotor. Radius corrections serve for more precise control RCF, exemplary when user need to know real RCF in half length of test tube. ▪ To change the rotor radius, select RADIUS [mm] with $\blacktriangle \blacktriangledown$ keys. ▪ Press SET. ▪ Set demanded value by pressing $\blacktriangle \blacktriangledown$. ▪ Press SET.
ACCELERATION	3	<input type="checkbox"/> THERM.CHAMB.																	
DECELERATION	3	<input type="checkbox"/> AUTOM.LID OPENING																	
RADIUS (mm)	120	<input type="checkbox"/> START DELAY																	
DENSITY (g/cm³)	1.5																		
TEMP.OFFSET(°C)	0																		
CHAMBER DEL.(min)	1																		
 <p>The display shows the following information:</p> <ul style="list-style-type: none"> SPEED: 2000 RCF: 496 TIME: 00:02:00 TEMP: 12°C +20 PROG: -- 11740/----- PARAM+ MENU+ 	<p>When radius correction is activated,  symbol is visible on the screen. Reducing of the rotor radius resulting change of displayed RCF value.</p>																		

9.3 Sample density
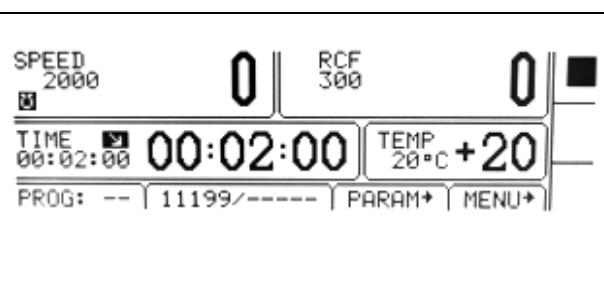
<p>PARAMETERS</p> <table border="0"> <tr> <td>ACCELERATION</td> <td>3</td> <td><input type="checkbox"/> THERM.CHAMB.</td> </tr> <tr> <td>DECELERATION</td> <td>3</td> <td><input type="checkbox"/> AUTOM.LID OPENING</td> </tr> <tr> <td>RADIUS (mm)</td> <td>120</td> <td><input type="checkbox"/> START DELAY</td> </tr> <tr> <td>DENSITY (g/cm³)</td> <td>1.5</td> <td></td> </tr> <tr> <td>TEMP.OFFSET(°C)</td> <td>0</td> <td></td> </tr> <tr> <td>CHAMBER DEL.(min)</td> <td>1</td> <td></td> </tr> </table>	ACCELERATION	3	<input type="checkbox"/> THERM.CHAMB.	DECELERATION	3	<input type="checkbox"/> AUTOM.LID OPENING	RADIUS (mm)	120	<input type="checkbox"/> START DELAY	DENSITY (g/cm³)	1.5		TEMP.OFFSET(°C)	0		CHAMBER DEL.(min)	1		<ul style="list-style-type: none"> ▪ DENSITY (g/cm³) – default density is set to 1,2 g/cm³ To change the density (possible values 1,2÷9,9 g/cm³): <ul style="list-style-type: none"> ▪ Via $\blacktriangle \blacktriangledown$ keys select DENSITY (g/cm³) ▪ Press SET. ▪ Set demanded value by pressing $\blacktriangle \blacktriangledown$. ▪ Press SET.
ACCELERATION	3	<input type="checkbox"/> THERM.CHAMB.																	
DECELERATION	3	<input type="checkbox"/> AUTOM.LID OPENING																	
RADIUS (mm)	120	<input type="checkbox"/> START DELAY																	
DENSITY (g/cm³)	1.5																		
TEMP.OFFSET(°C)	0																		
CHAMBER DEL.(min)	1																		
 <p>The display shows the following information:</p> <ul style="list-style-type: none"> SPEED: 2000 RCF: 300 TIME: 00:02:00 TEMP: 20°C +20 PROG: -- 11199/----- PARAM+ MENU+ 	<p>When density is changed,  symbol is visible on the screen. Changing of DENSITY value is obligatory when density of sample placed into rotor is higher than 1.2 g/cm³. Change of DENSITY value led to decreasing maximum value of accessible speed.</p>																		

9.4 Temperature offset

	<p>MPW-352R and MPW-352RH only</p>																		
<p>PARAMETERS</p> <table border="0"> <tr> <td>ACCELERATION</td> <td>3</td> <td><input type="checkbox"/> THERM.CHAMB.</td> </tr> <tr> <td>DECELERATION</td> <td>3</td> <td><input type="checkbox"/> AUTOM.LID OPENING</td> </tr> <tr> <td>RADIUS (mm)</td> <td>120</td> <td><input type="checkbox"/> START DELAY</td> </tr> <tr> <td>DENSITY (g/cm³)</td> <td>1.5</td> <td></td> </tr> <tr> <td>TEMP.OFFSET(°C)</td> <td>0</td> <td></td> </tr> <tr> <td>CHAMBER DEL.(min)</td> <td>1</td> <td></td> </tr> </table>	ACCELERATION	3	<input type="checkbox"/> THERM.CHAMB.	DECELERATION	3	<input type="checkbox"/> AUTOM.LID OPENING	RADIUS (mm)	120	<input type="checkbox"/> START DELAY	DENSITY (g/cm³)	1.5		TEMP.OFFSET(°C)	0		CHAMBER DEL.(min)	1		<p>Temperature offsets serve for more precise control of real sample temperature. It can be helpful in case high/low initial temperature samples or high-volume samples.</p> <ul style="list-style-type: none"> ▪ With $\blacktriangle \blacktriangledown$ keys select TEMP. OFFSET. ▪ Press SET. ▪ Use the $\blacktriangle \blacktriangledown$ keys to select the difference
ACCELERATION	3	<input type="checkbox"/> THERM.CHAMB.																	
DECELERATION	3	<input type="checkbox"/> AUTOM.LID OPENING																	
RADIUS (mm)	120	<input type="checkbox"/> START DELAY																	
DENSITY (g/cm³)	1.5																		
TEMP.OFFSET(°C)	0																		
CHAMBER DEL.(min)	1																		

	<p>between the temperature that the cooling system will aim for and set temperature. Confirm selection by pressing SET.</p> <p>Attention!</p> <p>The use of the offset cannot extend the temperature range achieved by the centrifuge.</p> <p>Function description</p> <p>At a set temperature of 20°C and the set offset value equal to -5°C, cooling system will actually strive to reach 15°C. With a setpoint temperature of 20°C and a set offset value of 5°C the system will actually try to reach 25°C. The temperature displayed on the main screen is corrected for offset value.</p> <p>Offset can be selected range from -20°C to 20°C.</p>
	<p>Activation of the function is signaled on the main screen with or depending on the offset value sign.</p>


9.5 Thermal chamber

	MPW-352R and MPW-352RH only
Cooling without centrifuging.	THERMAL CHAMBER
<p>PARAMETERS</p> <hr/> ACCELERATION 3 <input checked="" type="checkbox"/> THERM. CHAMB. DECELERATION 3 <input type="checkbox"/> AUTOM. LID OPENING RADIUS (mm) 120 <input type="checkbox"/> START DELAY DENSITY (g/cm³) 1.5 TEMP. OFFSET (°C) 0 CHAMBER DEL. (min) 1	<ul style="list-style-type: none"> With ▲▼◀▶ keys select THERMAL CHAMBER. Press SET (to turn on/off). With ▲▼ keys select temperature value. Set demanded value (0°C÷40°C) by pressing ▲▼. Confirm selection by pressing SET. Attention, in the centrifuge without heating, do not set the thermal chamber to a value higher than currently indicated by the centrifuge.
<p>SPEED 2000 RCF 537 0</p> <p>TIME 00:02:00 TEMP 5°C +20 T</p> <p>PROG: -- 11740/----- PARAM+ MENU+</p>	<ul style="list-style-type: none"> When THERMAL CHAMBER function is activated, symbol is visible on the screen. Changing temperature from the main screen is not possible. Opening cover terminates THERMAL CHAMBER function (closing cover back turns it on).
<p>PARAMETERS</p> <hr/> ACCELERATION 3 <input checked="" type="checkbox"/> THERM. CHAMB. DECELERATION 3 <input type="checkbox"/> AUTOM. LID OPENING RADIUS (mm) 120 <input type="checkbox"/> START DELAY DENSITY (g/cm³) 1.5 TEMP. OFFSET (°C) 0 CHAMBER DEL. (min) 1	<ul style="list-style-type: none"> Thermal chamber is activated with delay. Set time of delaying by select CHAMBER DEL.. Press SET. With ▲▼ keys select demanded value (1-5 min). Press SET.


- The function is activated automatically after confirmation and with the lid closed. When the lid is opened, the function is interrupted, and when the lid is closed again, the function resumes. If the **THERMAL CHAMBER** function is enabled during the centrifugation cycle, at the end of this cycle, the **THERMAL CHAMBER** function is activated until the lid is opened.
- Contrary to other parameters, the **THERMAL CHAMBER** function can be turned on only when the centrifuge is stopped.

9.6 Automatic lid opening

Automatic lid opening	AUTOMATIC LID OPENING
PARAMETERS <hr/> ACCELERATION 3 <input type="checkbox"/> THERM.CHAMB. DECELERATION 3 <input type="checkbox"/> AUTOM.LID OPENING RADIUS (mm) 120 <input type="checkbox"/> START DELAY DENSITY (g/cm³) 1.5 TEMP.OFFSET(°C) 0 CHAMBER DEL.(min) 1	<ul style="list-style-type: none"> When centrifuge process is finished, cover will be opened automatically for set option AUTOM. LID OPENING. When centrifuging is terminated by pressing STOP, opening cover is possible by pressing COVER.

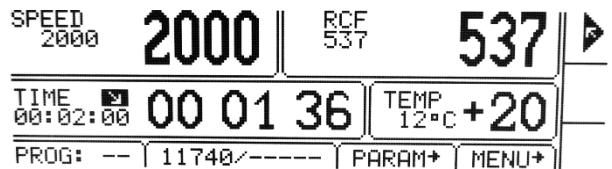	<ul style="list-style-type: none"> ► symbol means that OPEN LID AFTER RUN is active.
--	---

9.7 Start delay - of time

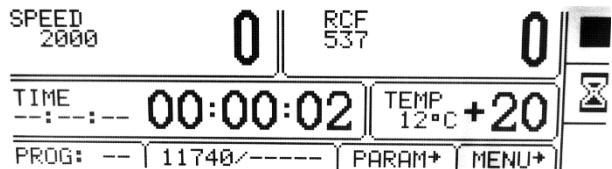 Start centrifuging since preselected delay is reached.	STARY DELAY / OF TIME
PARAMETERS <hr/> ACCELERATION 3 <input type="checkbox"/> THERM.CHAMB. DECELERATION 3 <input type="checkbox"/> AUTOM.LID OPENING RADIUS (mm) 120 <input type="checkbox"/> START DELAY DENSITY (g/cm³) 1.2 <input type="checkbox"/> OF TIME 0:00:01 TEMP.OFFSET(°C) 0 <input type="checkbox"/> OF TEMP 7°C CHAMBER DEL.(min) 1	<ul style="list-style-type: none"> With ▲▼ keys select START DELAY. Press SET. Start delay can be set from 0 : 0 0 : 0 1 to 9 : 5 9 : 5 9. With ▲▼ keys select OF TIME. Press SET and ► and then SET. With ▲▼ keys set demanded value. Confirm by pressing SET. Press BACK to escape edit mode.
	<ul style="list-style-type: none"> Start delay – the time is illustrated by a flashing symbol ☰.

▪ START DELAY / **OF TIME** function cannot be run when START DELAY / **OF TEMP**. is activated.

9.8 Start delay – of temperature



MPW-352R and MPW-352RH only

	Start centrifuging time counting since preselected temperature is reached.	START DELAY / OF TEMP.
PARAMETERS	<pre> ACCELERATION 3 □ THERM. CHAMB. DECELERATION 3 □ AUTOM. LID OPENING RADIUS (mm) 120 □ START DELAY DENSITY (g/cm³) 1.2 □ OF TIME 0:00:01 TEMP.OFFSET(°C) 0 □ OF TEMP 7°C CHAMBER DEL.(min) 1 </pre>	<ul style="list-style-type: none"> With ▲▼◀▶ keys mark START DELAY. Press SET. With ▲▼◀▶ keys mark OF TEMP. Press SET. Press ▶, press SET. With ▲▼ keys set demanded value of temperature. Press SET. Exit edit mode by press BACK.
		<ul style="list-style-type: none"> When START DELAY – OF TEMPERATURE is turned on, symbol is visible on the screen.
When the function is active, the speed can be reduced to the optimum values for the FAST COOL function, when the set speed is lower than the optimum value, the rotor rotates at the set by user speed.		START DELAY / OF TEMP. function cannot be run when START DELAY / OF TIME is activated.

10 Menu

Simplified display	<ul style="list-style-type: none"> Press and hold BACK by 1 second. Choose MENU with ▲▼ Press SET. Execute points described follow (below Normal display mode description)
Normal display	<ul style="list-style-type: none"> Press SET. With ▲▼◀▶ keys select MENU. Press SET.

MENU	
CONFIGURATION PASSWORD LAST 10 CYCLES WORK TIME	ROTOR RUNTIME CONTACT US DIAGNOSTICS FACTORY SETTINGS

CONFIGURATION	centrifuge configuration
PASSWORD	password protection
LAST 10-CYCLES	10 last centrifugation cycles history
CYCLES	total working time of centrifuge, total number of working cycles counter
ROTOR RUNTIME	counting time of work and cycles amount for each rotor
CONTACT US	manufacturer's details
DIAGNOSTICS	error codes (service field)
FACTORY SETTINGS	restore factory settings

10.1 Screen saver

Setting time of screen saver	MENU/ CONFIGURATION / SCREEN
<p>SCREEN \leftrightarrow 1/5</p> <p><input checked="" type="checkbox"/> SCREENSAVER: 15 min <input type="checkbox"/> VISUAL ALARM <input type="checkbox"/> NORMAL DISPLAY <input type="checkbox"/> SIMPLIFIED DISPLAY</p>	<ul style="list-style-type: none"> With $\blacktriangle\blacktriangledown\blackleftarrow\blackrightarrow$ keys select SCRENSAVER. Press SET and then \blacktriangledown and SET . With $\blacktriangle\blacktriangledown$ keys select demanded value from 1 to 60 minutes. Mark selection by pressing SET. Leave the menu by pressing BACK.

10.2 Visual alarm

Visual alarm	MENU/CONFIGURATION/ SCREEN
<p>SCREEN \leftrightarrow 1/5</p> <p><input checked="" type="checkbox"/> SCREENSAVER: 15 min <input type="checkbox"/> VISUAL ALARM <input type="checkbox"/> NORMAL DISPLAY <input type="checkbox"/> SIMPLIFIED DISPLAY</p>	<ul style="list-style-type: none"> Via $\blacktriangle\blacktriangledown$ keys choose VISUAL ALARM Mark it by pressing SET. <p>VISUAL ALARM cause blinking screen after ending of centrifuging or after message occurring.</p>

10.3 Types of main screen

To ensure optimal adaptation to the user's preferences, work is possible in two basic screen modes.

NORMAL DISPLAY - contains an expanded number of parameters visible on the display.

SIMPLIFIED DISPLAY - contains only the most important parameters visible on the display.


For each of the above modes, you can choose priority RPM display or RCF.

By default, the **SIMPLIFIED DISPLAY** is set.


Types of main screen	
	
Switch between the SPEED (RPM) and RCF display priority modes	

- In the **NORMAL DISPLAY** mode, selecting the **SPEED** or **RCF** display mode is obtained by pressing and holding **BACK** for 1 sec.
- then use the **▲ ▼** buttons to select the desired mode (**SPEED** or **RCF**) and press **SET**.
- In the **SIMPLIFIED DISPLAY** mode, the selection of the **SPEED** or **RCF** display mode is obtained by pressing and holding the **BACK** key for 1 second.
- then use **▲ ▼** keys to select **DISPLAY MODE**, press **SET**, and then use **▲ ▼** keys to select the desired mode (**SPEED** or **RCF**) and press **SET**.

10.3.1 Switching the normal display to simplified display

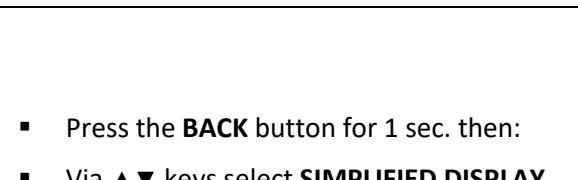	
<ul style="list-style-type: none"> ▪ Press the BACK button for 1 sec. then: ▪ Via ▲ ▼ keys select SIMPLIFIED DISPLAY. ▪ Press SET. 	

10.3.2 Switching the simplified screen to normal display

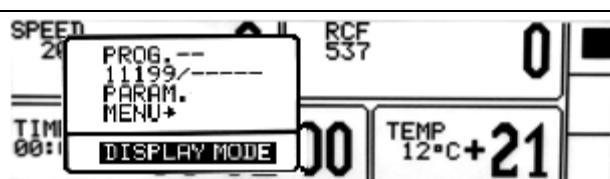	<ul style="list-style-type: none"> ▪ Press the BACK button for 1 sec. then:
	<ul style="list-style-type: none"> ▪ Via ▲ ▼ keys select DISPLAY MODE (blinking). ▪ Press SET. ▪ Then choose NORMAL DISPLAY and press SET.

10.4 Rotating runtime

Way of time counting	MENU/CONFIGURATION/ ROTATING RUNTIME
ROTATING RUNTIME ↔ 2/5 <input checked="" type="checkbox"/> COUNTING FROM PRESSING START <input type="checkbox"/> COUNTING FROM REACHING SPEED <input type="checkbox"/> DESCENDING <input type="checkbox"/> ASCENDING	<ul style="list-style-type: none"> ▪ Via ▲ ▼ choose demanded option. ▪ Mark it by pressing SET.

Counting from:	
Pressing start →	Counting since rotor is identified
Reaching speed →	Counting from assigned speed
Presenting mode:	
Descending →	Counting down
Ascending →	Counting up

10.5 Buzzer

Switching ON/OFF short audible signals accompanying every pressing of any key. Switching ON/OFF signals after centrifuging.	MENU/ CONFIGURATION /BUZZER
BUZZER <hr/> <input type="checkbox"/> KEY TONE <input type="checkbox"/> CONTINUOUS ALARM	<ul style="list-style-type: none"> ▪ With ▲▼ keys select demanded option. ▪ Mark selection by pressing SET. A continuous alarm means the emission of short beeps after the end of the spin, until the message about the end of the work cycle is deleted.
Warning signals are always switched on.	

10.6 Date/time*

Setting up time and date	MENU/ CONFIGURATION /DATE/TIME						
DATE/TIME <hr/> <table style="width: 100%;"><tr><td style="width: 50%;">DATE</td><td style="width: 50%;">TIME</td></tr><tr><td>DD-MM-YYYY</td><td>HH:MM:SS</td></tr><tr><td>05-01-2017</td><td>18:48:11</td></tr></table>	DATE	TIME	DD-MM-YYYY	HH:MM:SS	05-01-2017	18:48:11	<ul style="list-style-type: none"> ▪ Press SET. ▪ Via ◀▶ keys choose demanded value. ▪ Via ▲▼ keys change chosen value. ▪ Confirm by pressing SET. ▪ Repeat above steps for other values. ▪ Press BACK.
DATE	TIME						
DD-MM-YYYY	HH:MM:SS						
05-01-2017	18:48:11						
Set date and time are still active even after restart of centrifuge.							


10.7 Language

Changing menu language	MENU / CONFIGURATION / LANGUAGE										
LANGUAGE <hr/> <table style="width: 100%;"><tr><td style="width: 50%;"><input type="checkbox"/> POLSKI</td><td style="width: 50%;"><input type="checkbox"/> DEUTSCH</td></tr><tr><td><input checked="" type="checkbox"/> ENGLISH</td><td><input type="checkbox"/> РУССКИЙ</td></tr><tr><td><input type="checkbox"/> ESPANOL</td><td><input type="checkbox"/> SVENSKA</td></tr><tr><td><input type="checkbox"/> ITALIANO</td><td><input type="checkbox"/> FRANCAIS</td></tr><tr><td><input type="checkbox"/> PORTUGUES</td><td><input type="checkbox"/> ČESKÝ</td></tr></table>	<input type="checkbox"/> POLSKI	<input type="checkbox"/> DEUTSCH	<input checked="" type="checkbox"/> ENGLISH	<input type="checkbox"/> РУССКИЙ	<input type="checkbox"/> ESPANOL	<input type="checkbox"/> SVENSKA	<input type="checkbox"/> ITALIANO	<input type="checkbox"/> FRANCAIS	<input type="checkbox"/> PORTUGUES	<input type="checkbox"/> ČESKÝ	<ul style="list-style-type: none"> ▪ Via ▲▼ keys choose demanded menu language ▪ Mark it by pressing SET.
<input type="checkbox"/> POLSKI	<input type="checkbox"/> DEUTSCH										
<input checked="" type="checkbox"/> ENGLISH	<input type="checkbox"/> РУССКИЙ										
<input type="checkbox"/> ESPANOL	<input type="checkbox"/> SVENSKA										
<input type="checkbox"/> ITALIANO	<input type="checkbox"/> FRANCAIS										
<input type="checkbox"/> PORTUGUES	<input type="checkbox"/> ČESKÝ										

* In selected models the function is not available.


10.8 Other

10.8.1 Rotor automatic identification



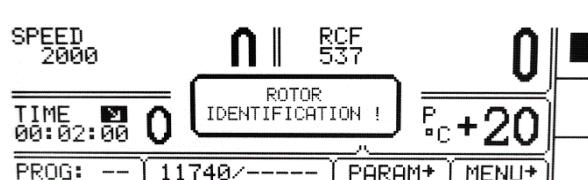
MENU / CONFIGURATION / OTHER	
<p>OTHER ↔ 5/5</p> <p><input checked="" type="checkbox"/> AUTOMATIC IDENTIF. <input type="checkbox"/> TEMPERATURE: °C <input type="checkbox"/> TEMPERATURE: °F</p>	<p>Thanks to the automatic rotor identification, the centrifuge automatically identifies the rotor in the chamber. Rotor identification is indicated by the message.</p> <p>When the function is deactivated, it is necessary to manually select the desired rotor as described in "Choosing rotors".</p> <p>The AUTOMATIC IDENTIF. is turned on by default.</p> <p>To enable/disable the function:</p> <ul style="list-style-type: none"> ▪ Via ▲▼ keys choose <input checked="" type="checkbox"/> AUTOMATIC IDENTIF. ▪ Press SET (<input type="checkbox"/> change to <input checked="" type="checkbox"/> or conversely). <p>Autoidentification is not active for work in the loaded program mode.</p>
<p>OTHER ↔ 6/6</p> <p><input checked="" type="checkbox"/> AUTOMATIC IDENTIF. <input type="checkbox"/> TEMPERATURE: °C <input type="checkbox"/> TEMPERATURE: °F <input type="checkbox"/> SERVICE INSPECTION</p> <p>Screen view available on models with the Date/Time function enabled</p>  <p>SPEED 2000 RCF 537 TIME 00:02:00 ROTOR IDENTIFICATION! TEMP 12°C +21 PROG: -- 11740/----- PARAM+ MENU+</p>	

10.8.2 Selecting the temperature unit


Choice of temperature unit	MENU / CONFIGURATION / OTHER
<p>OTHER ↔ 5/5</p> <p><input checked="" type="checkbox"/> AUTOMATIC IDENTIF. <input type="checkbox"/> TEMPERATURE: °C <input type="checkbox"/> TEMPERATURE: °F</p>	<p>The TEMPERATURE in °C is turned on by default.</p>
<p>OTHER ↔ 6/6</p> <p><input checked="" type="checkbox"/> AUTOMATIC IDENTIF. <input type="checkbox"/> TEMPERATURE: °C <input type="checkbox"/> TEMPERATURE: °F <input type="checkbox"/> SERVICE INSPECTION</p> <p>Screen view available on models with the Date/Time function enabled</p>	<p>To change the temperature unit:</p> <ul style="list-style-type: none"> ▪ Via ▲▼ keys select unit ▪ Confirm by pressing SET.

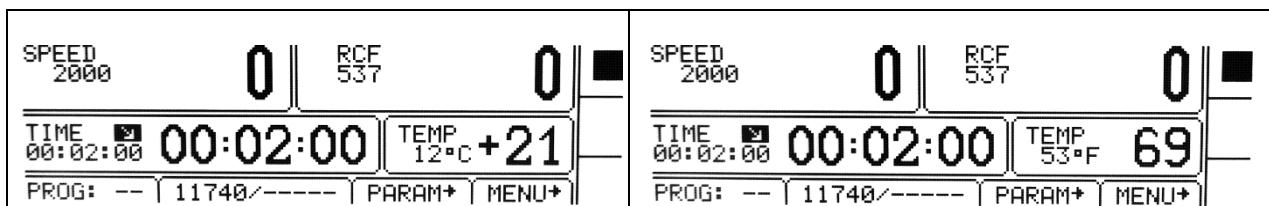

10.8.3 Service inspection*

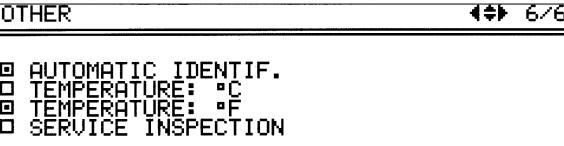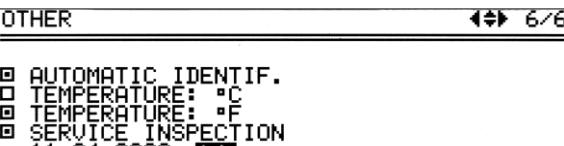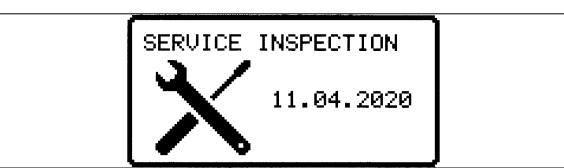	MENU / CONFIGURATION / OTHER
  	<p>There is a possibility to turn on a message reminding user to perform the inspection, with the option to define the date of the inspection when the message will be displayed.</p> <p>To enable/unable the function:</p> <ul style="list-style-type: none"> ▪ Via ▲▼ keys choose <input type="checkbox"/> SERVICE INSPECTION. ▪ Press SET (<input type="checkbox"/> change to <input checked="" type="checkbox"/> or conversely). <p>A new field will appear with the date of the inspection (on that day message will be displayed).</p> <p>To edit the date:</p> <ul style="list-style-type: none"> ▪ Via ▲▼ keys select date field. ▪ Press SET. ▪ Via ▲▼◀▶ keys choose value. ▪ Confirm by pressing SET.

10.9 Password

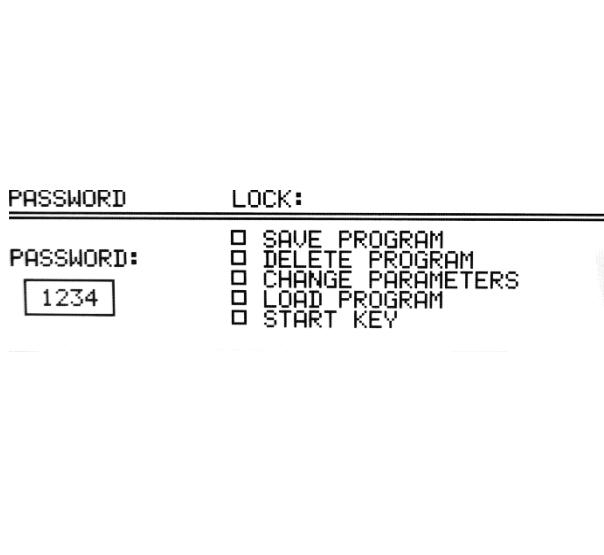Setting up password	MENU / PASSWORD
<p>To prevent from an unauthorized use, a PASSWORD can be set.</p> <p>Note: No PASSWORD is set by default.</p> <p>The PASSWORD can be set as follows when the rotor is at a standstill.</p> 	<ul style="list-style-type: none"> ▪ With ▲▼ keys select the PASSWORD field (is blinking), press SET. ▪ With the ▲▼ keys select the appropriate digit in the first field, e.g., 1xxx. ▪ Press ▶ ▪ With the ▲▼ keys select the appropriate digit in the second field, e.g., 12xx. ▪ Press ▶ ▪ Use the ▲▼ keys to select the appropriate digit in the third field, e.g., 123x. ▪ Press ▶ ▪ Use the ▲▼ keys to select the correct digit in the fourth field, e.g., 1234. ▪ Press SET.

* This function is only available in models with the **Date/Time** tab active.

PASSWORD	LOCK:	
CONFIRM: 1234	<input type="checkbox"/> SAVE PROGRAM <input type="checkbox"/> DELETE PROGRAM <input type="checkbox"/> CHANGE PARAMETERS <input type="checkbox"/> LOAD PROGRAM <input type="checkbox"/> START KEY	<ul style="list-style-type: none"> ▪ As a confirmation repeat instructions described above.

When the **PASSWORD** is set, the Key sign is displayed in the **CODE** zone. It is also displayed in the main menu (lower right corner of the screen).

PASSWORD	LOCK:	SPEED 2000	RCF 300	0	0	■
****	<input type="checkbox"/> SAVE PROGRAM <input type="checkbox"/> DELETE PROGRAM <input type="checkbox"/> CHANGE PARAMETERS <input type="checkbox"/> LOAD PROGRAM <input type="checkbox"/> START KEY	TIME 00:02:00	00:02:00	TEMP 20°C +20	PROG: --- T 11199/----- T PARAM+ T MENU+	PF

From then on, access to the **MENU** is possible after entering the password.

In case of incorrect password, it will show message: **ACCESS DENIED!**

The removal of an active password is possible after setting the password "**0000**" (after entering the currently set password). If the password is forgotten, it is possible to use the emergency password "**7654**", which removes the previous password and all locks. Using both methods will delete the previous password and disable all security features.

Setting up locks

PASSWORD	LOCK:	<ul style="list-style-type: none"> ▪ With ▲▼ keys choose a lock. ▪ Mark a lock by pressing SET. ▪ Repeat above steps for desired locks. ▪ Leave menu with BACK key.
****	<input type="checkbox"/> SAVE PROGRAM <input type="checkbox"/> DELETE PROGRAM <input type="checkbox"/> CHANGE PARAMETERS <input type="checkbox"/> LOAD PROGRAM <input type="checkbox"/> START KEY	

	Disabled*	description
SAVE PROGRAM	button	<ul style="list-style-type: none"> ▪ no programs can be saved
DELETE PROGRAM	button	<ul style="list-style-type: none"> ▪ no programs can be deleted ▪ saving programs on position where one was already stored is disabled
CHANGE PARAMETERS	fields: SPEED RCF TIME TEMP PROG— — / — PARAM PROG	<ul style="list-style-type: none"> ▪ parameters cannot be modified
LOAD PROGRAM	button	<ul style="list-style-type: none"> ▪ no programs can be called up
START KEY	key	<ul style="list-style-type: none"> ▪ centrifugation cannot be started

* Executing disabled procedures is only possible after entering the correct

10.10 Last 10 cycles

Information concerning parameters of last 10 centrifuging cycles.	MENU / LAST 10 CYCLES
<pre>NO CYCLES:05 ◀▶ DATE/TIME: 2017.01.05/ 18:18 PROGRAM: -- ROTOR/BUCKET: 11740/----- SPEED: 2000 RCF: 537 TIME: 00:02:00</pre>	<ul style="list-style-type: none"> ▪ Number of cycles can be changed by ◀▶ keys. ▪ The list can be scrolled using ▲▼ keys. ▪ To exit press SET/BACK key

10.11 Work time

Total working time of centrifuge, and quantity of working cycles.	MENU / WORK TIME
<p>WORK TIME</p> <hr/> <p>TOTAL RUN TIME: 0h 13m 14s</p> <p>CYCLES: 31</p>	<p>In the WORK TIME menu, the following statistics are displayed:</p> <ul style="list-style-type: none"> ▪ total working (centrifugation) time ▪ working cycles counter

10.12 Rotor runtime

Information about the time of centrifuging and of the quantity of the working cycles of each rotor. The table also contains icons warning of the duty of execution of validation.	MENU / ROTOR RUNTIME																																																	
<table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th>No</th> <th>S</th> <th>ROTOR</th> <th>BUCKET</th> <th>CYCLES</th> <th>NOM.C</th> <th>TIME</th> </tr> </thead> <tbody> <tr> <td>1</td> <td>✓</td> <td>11199</td> <td>-----</td> <td>1</td> <td>15000</td> <td>0</td> </tr> <tr> <td>2</td> <td>✓</td> <td>11210</td> <td>-----</td> <td>0</td> <td>15000</td> <td>0</td> </tr> <tr> <td>3</td> <td>✓</td> <td>11211</td> <td>-----</td> <td>0</td> <td>15000</td> <td>0</td> </tr> <tr> <td>4</td> <td>✓</td> <td>11213</td> <td>-----</td> <td>0</td> <td>15000</td> <td>0</td> </tr> <tr> <td>5</td> <td>✓</td> <td>11259</td> <td>-----</td> <td>0</td> <td>15000</td> <td>0</td> </tr> <tr> <td>6</td> <td>✓</td> <td>11273</td> <td>-----</td> <td>0</td> <td>15000</td> <td>0</td> </tr> </tbody> </table>	No	S	ROTOR	BUCKET	CYCLES	NOM.C	TIME	1	✓	11199	-----	1	15000	0	2	✓	11210	-----	0	15000	0	3	✓	11211	-----	0	15000	0	4	✓	11213	-----	0	15000	0	5	✓	11259	-----	0	15000	0	6	✓	11273	-----	0	15000	0	<ul style="list-style-type: none"> ▪ The list can be scrolled using ▲▼ keys. ▪ To exit press BACK key. <p>Symbols:</p> <p>✓ – more than 100 cycles left !! – less than 100 cycles left █ – worn rotor</p> <p>It is not allowed to use rotors marked as worn. They should be replaced with new ones.</p>
No	S	ROTOR	BUCKET	CYCLES	NOM.C	TIME																																												
1	✓	11199	-----	1	15000	0																																												
2	✓	11210	-----	0	15000	0																																												
3	✓	11211	-----	0	15000	0																																												
4	✓	11213	-----	0	15000	0																																												
5	✓	11259	-----	0	15000	0																																												
6	✓	11273	-----	0	15000	0																																												

10.13 Contact us

Information about the type of the centrifuge, firmware version, and contact details.	MENU / CONTACT US
<p>CONTACT US MPW-352R v7.9.16 ◀▶</p> <p>MPW MED. INSTRUMENTS 04-347 WARSAW 46 BOREMLOWSKA STREET WWW.MPW.PL , MPW@MPW.PL SALES DEPARTMENT:</p>	<ul style="list-style-type: none"> ▪ The list can be scrolled using ▲▼ keys. ▪ To exit press BACK key.

10.14 Diagnostics

Information about errors arisen in working of the centrifuge (for service).	MENU / DIAGNOSTICS																																			
<table border="1"> <thead> <tr> <th>NO</th> <th>DATE</th> <th>TIME</th> <th>ERROR</th> <th>▼</th> </tr> </thead> <tbody> <tr> <td>2</td> <td>► 05.01.2017</td> <td>18:12</td> <td>200</td> <td></td> </tr> <tr> <td>3</td> <td></td> <td></td> <td></td> <td></td> </tr> <tr> <td>4</td> <td></td> <td></td> <td></td> <td></td> </tr> <tr> <td>5</td> <td></td> <td></td> <td></td> <td></td> </tr> <tr> <td>6</td> <td></td> <td></td> <td></td> <td></td> </tr> <tr> <td>7</td> <td></td> <td></td> <td></td> <td></td> </tr> </tbody> </table> <p>Screen view available on models with the Date/Time function enabled</p>	NO	DATE	TIME	ERROR	▼	2	► 05.01.2017	18:12	200		3					4					5					6					7					Intended for service purposes!
NO	DATE	TIME	ERROR	▼																																
2	► 05.01.2017	18:12	200																																	
3																																				
4																																				
5																																				
6																																				
7																																				

10.15 Factory settings

Restoring factory settings.	MENU/ FACTORY SETTINGS
<p>All settings of user programs will be deleted.</p> <p>FACTORY SETTINGS: WARNING! ALL PROGRAMS, SETTINGS AND CONFIGURATION WILL BE LOST. CONTINUE ?</p> <p>YES NO</p>	<ul style="list-style-type: none"> ▪ Via ►► keys choose YES or NO. ▪ Confirm by pressing SET.

11 Maintenance

11.1 Cleaning of the centrifuge

	<ul style="list-style-type: none"> ▪ Pull the mains plug before cleaning. ▪ Before any cleaning or decontamination process other than that is recommended by the manufacturer, the user has to ask the manufacturer if the planned process does not damage the device ▪ For cleaning, water with soap or other water-soluble mild detergent shall be used. ▪ One should avoid corrosive and aggressive substances. ▪ It is prohibited to use alkaline solutions, inflammable solvents or agents containing abrasive particles. ▪ Do not lubricate the centrifuge motor shaft. ▪ The unused centrifuge should have cover opened. <p style="text-align: center;">Once a week</p> <ul style="list-style-type: none"> ▪ Using wiping cloth, remove condensate or residues of the products from the rotor chamber. <p style="text-align: center;">Once a month</p> <ul style="list-style-type: none"> ▪ Check the condition of the rotor fixing screw thread. If damaged, it must be replaced. ▪ Check the centrifuging chamber whether it is damaged. In case of damage, it cannot be longer put into operation. Notify authorized service workshop.

11.2 Maintenance of centrifuge elements

	<ul style="list-style-type: none"> ▪ The rotor pins shall be always lubricated with petroleum jelly. ▪ In this way, the uniform deflection of the buckets and quiet centrifuge operation is ensured.
---	--

Cleaning of the equipment

	<ul style="list-style-type: none"> ▪ In order to ensure safe operation, one shall carry out in regular way periodical maintenance of the equipment. ▪ Rotors, buckets, and round carriers have to withstand high stresses originating from the centrifugal force. Chemical reactions as well as corrosion (combination of variable pressure and chemical reactions) can cause destruction of metals. Hard to observe surface cracks increase gradually and weaken material without visible symptoms. ▪ In case of observation of surface damage, crevice, or other change, as well as the corrosion, the given part (rotor, bucket, etc.) shall be immediately replaced. ▪ The rotor, including the fixing screw, buckets and round carriers must be regularly cleaned to prevent corrosion. ▪ Cleaning of the accessories shall be carried out outside of the centrifuge once every week or still better after each use. For cleaning them one should use neutral agent of pH value 6÷8. It is forbidden to use alkaline agent of pH > 8. Then, those parts shall be dried using soft fabric or in the chamber drier at ca. 50°C. ▪ Angle rotor should be placed on a fabric with holes facing down, for effective drying. ▪ Do not use bleach on plastic parts of the rotor. ▪ In this way, the useful service life of the device is substantially increased and susceptibility to corrosion is diminished. Accurate maintenance increases the service life as well and protects against premature rotor failures. ▪ Do not use bleach on plastic parts of the rotor. ▪ According to laboratory standards, minimize the immersion time in each solution. ▪ Especially prone to the corrosion are parts made of aluminium. ▪ Corrosion and damages resulting from insufficient maintenance could not be subject of claims lodged against the manufacturer. ▪ The unused rotor should have the lid removed.
---	--

- HS accessories maintenance.

	<ul style="list-style-type: none"> ▪ Check the general condition of seals. ▪ Make sure that rubber O-rings are lightly coated with silicone grease. Use high vacuum grease, e.g., type „C” by LUBRINA. ▪ In order to maintain hermetic sealing, it is recommended to replace the sealing rings after each autoclaving. ▪ Store hermetically sealed rotors and buckets with the lids removed.
---	--

11.3 Sterilization

Plastics - legend to abbreviations

PS	polystyrene	ECTFE	ethylene/chlorotrifluoroethylene
SAN	styrene-acrylonitrile	ETFE	ethylene/tetrafluoroethylene
PMMA	polymethyl methacrylate	PTFE	polytetrafluoroethylene
PC	polycarbonate	FEP	tetrafluoroethylene/perfluoropropylene
PVC	polyvinyl chloride	PFA	tetrafluoroethylene/perfluoroalkylvinylether
POM	acetal polyoxymethylene	FKM	fluorcarbon rubber
PE-LD	low density polyethylene	EPDM	ethylene propylene diene
PE-HD	high density polyethylene	NR	natural rubber
PP	polypropylene	SI	silicon rubber
PMP	polymethylpentene		

One can use all standard disinfectants. Centrifuges and devices are made of different materials, one should consider their variety.

	radiation β radiation γ 25 kGy	C_2H_4O (ethylene oxide)	formalin, ethanol
PS	●	○	●
SAN	○	●	●
PMMA	●	○	●
PC	●	●	●
PVC	○	●	●
POM	●	●	●
PE-LD	●	●	●
PE-HD	●	●	●
PP	●	●	●
PMP	●	●	●
ECTFE, ETFE	○	●	●
PTFE	○	●	●
FEP, PFA	○	●	●
FKM	○	●	●
EPDM	○	●	●
NR	○	●	●
SI	○	●	●

● may be used

○ cannot be used

In the centrifuge, disinfectants and cleaning agents generally used in medical care should be used (e.g., Aerodesina-2000, Lysoformin 3000, Melseptol, Melsept SF, Sanepidex, Cutasept F).

11.3.1 Autoclaving

- Rotors, buckets, and round carriers can be sterilized in autoclave with temperature 121°C during 20 min (215 kPa), unless otherwise specified in the OPTIONAL ACCESSORY.
- During sterilization (autoclaved) by means of steam one should consider temperature resistance of individual materials.
- Deformation of the accessories (carriers or lids made of plastic) may occur during autoclaving.
- Do not autoclave disposable materials (e.g., tubes, cyto-container).
- The life of the accessory depends on the frequency of autoclaving and use.
- Autoclaving reduces lifespan of plastic components. They should be replaced if any signs of damage are visible, including a change in colour or shape or when leakage etc.
- Pressure in closed containers can cause plastic deformation or explosion.
- Prior to autoclaving the rotors and accessories, thoroughly wash and rinse with distilled water.
- Never exceed the permissible autoclaving temperature and time.
- If you want to keep the hermetic seals, replace the sealing rings after each autoclave.

Chemical resistance of plastics

	autoclaving 121 °C, 20 min		autoclaving 121 °C, 20 min
PS	○	PMP	●
SAN	○	ECTFE, ETFE	●
PMMA	○	PTFE	●
PC	●	FEP, PFA	●
PVC	○ ¹⁾	FKM	●
POM	●	EPDM	●
PE-LD	○	NR	○
PE-HD	○	SI	●
PP	●		

- may be used
 - cannot be used
- 1) Except PVC hoses which are resistant to the steam sterilization in the temperature 121°C.

11.4 Chemical resistance

Chemical resistance of plastics

	aldehydes	cyclic alcohols	esters	ether	ketones	strong or concentrated acids	weak or diluted acids	oxidizing substances	cyclic hydrocarbons	ahs	haloid hydrocarbons	alkalis
PS	○	●	○	○	○	○/●	○/●	○	○	○	○	●
SAN	○	●	○	○	○	○	○/●	○	○	○	○	●
PMMA	○/●	●	○	○	○	○	○/●	○	○/●	○	○	○
PC	○/●	●	○	○	○	○	○/●	○	○/●	○	○	○
PVC	○	●	○	○	○	●	●	○	●	○	○	●
POM	○/●	●	○	●	●	○	○	○	●	●	●	●
PE-LD	●	●	●	●	○/●	●	●	○	●	●	●	●
PE-HD	●	●	○/●	○/●	○/●	●	●	○	●	○/●	○/●	●
PP	●	●	○/●	○/●	○/●	●	●	○	●	○/●	○/●	●
PMP	○/●	●	○/●		○/●	●	●	○	○/●	○	○	●
ECTFE ETFE	●	●	●	●	○	●	●	●	●	●	●	●
PTFE FEP PFA	●	●	●	●	●	●	●	●	●	●	●	●
FKM	●	○	○	○	○	○	●	○/●	○/●	○/●	○/●	○/●
EPDM	●	●	○/●	○	○/●	●	●	○/●	○	○	○	●
NR	○/●	●	○/●	○	○	○	○/●	○	○	○	○	●
SI	○/●	●	○/●	○	○	○	○/●	○	○	○	○	○/●
● very good			Permanent action of the substance does not cause damage through 30 days. The material is able to be resistant through years									
○/● good to limited			Continuous action of the substance causes insignificant and partly reversible damage through the period of 7-30 days (e.g., puffing up, softening, reduced mechanical durability, discolouring).									
○ limited			The material should not have the continuous contact with the substance. The immediate occurrence of damage is possible (e.g., the loss of mechanical durability, deformation, discolouring, bursting, dissolving).									

Rubber inserts shall be exactly cleaned or possibly replaced. Centrifuges and accessories are made of different materials.

Do not use bleach on plastic parts of the rotor.

	DANGER! MPW accessories are not biotight. For centrifuging infectious materials, it is necessary to use hermetically closed tubes meeting demands of biotightness, in order to prevent germs migration into the centrifuge and beyond it.
	User is responsible for proper disinfections of the centrifuge if some dangerous material was spilled inside or outside of the centrifuge. During the above mentioned works one must wear safety gloves.

12 Troubleshooting

Majority of faults could be removed by switching the centrifuge OFF and then ON. After switching the centrifuge ON, there shall be displayed parameters of the recently implemented program and sound signals comprising four successive tones shall be generated. In case of short-duration power failure the centrifuge terminates the cycle and displays PROGRAM ERROR code.

problem	question	remedy
Centrifuge does not start	<i>Is supply cable plugged into mains?</i>	<i>Plugs supply cable correctly.</i>
	<i>Is master switch ON?</i>	<i>Switch ON power supply.</i>
<i>Motor error is displayed</i>		
(indications are proof for cycle in progress and motor does not start)	<i>Is ► symbol displayed?</i>	Wait till rotor stops and the ► symbol goes off.
	<i>Is └ symbol displayed?</i>	Close cover. └ symbol must switch off.
	<i>Is ■ symbol blinking?</i>	Centrifugation cycle in progress, press STOP key or wait till cycle ends.
Centrifuge does not accelerate <i>(unbalance error)</i>	<i>Unequal rotor load.</i>	Centrifuge load shall be balanced.
	<i>Inclined centrifuge.</i>	Centrifuge shall be levelled.
	<i>Faulty drive (mechanical damage).</i>	Call service.
	<i>Was centrifuge displaced during operation?</i>	Switch ON the centrifuge again after opening and closing the cover.
<i>(motor error)</i>	<i>After stopping error rotor message is displayed</i>	Check if rotor number in started program is consistent with the number of the rotor installed in the centrifuge. Check rotor status (if there are coding magnets inserted)
	<i>Centrifuge does not recognize the rotor and does not stop.</i>	Switch the centrifuge OFF, then ON and check correctness of loaded program
<i>It is not possible to open the cover</i>	<i>■ symbol on the display is blinking, after pressing COVER key single tone is audible</i>	Rotor is still rotating. Wait for stopping of the rotor and displaying of the ■ symbol.
	<i>The sensor is connected correctly, and the error is still applying.</i>	Call service.
<i>Mains failure during run</i>	<i>The message will be displayed on the display about the decay of tension.</i>	Wait for stopping of the rotor, clear the error by pressing the SET key.
<i>Temperature sensor error</i>	<i>The overheating message will be displayed.</i>	Switch the centrifuge OFF, then ON.
		Call service.
<i>Error of the exceeding the temperature (50°C) in the chamber</i>	<i>The overheating message will be displayed.</i>	Call service.

12.1 Messages

Screen messages that may occur during operation.	
MESSAGE	EXPLANATION
"SPEED OF ROTOR" "IDENTIFICATION <> 90 RPM"	Please try start centrifuging again, if error still occur, contact manufacturer's authorized service.
"IMBALANCE FAST STOP!" "PLEASE REMOVE CAUSE" "THEN RESTART"	Rotor is not balanced correctly, please balance rotor.
"NO ROTOR OR IDENTIFICATION" "SENSOR DAMAGED!"	Make sure, is rotor mounted in the centrifuge chamber. If it is right contact manufacturer's authorized service.

"INCORRECT ROTOR NUMBER!"	Change rotor number in centrifuge settings or use autoidentification.
"WRONG DIRECTION OF ROTATION" "OR UNKNOWN ROTOR!"	Make sure if correct rotor for centrifuge is mounted. List of accessories is described in chapter 15.
"PLEASE CLOSE THE LID" "HAND!"	Necessity of manually closing the lid.
"ROTOR STOPPING!" "Please wait..."	Initializing after mains failure with rotating rotor, wait until rotor stop.

Emergency messages

In case of emergency messages (centrifuge is not working properly) contact the manufacturer's authorized service centre.

MESSAGE
"OVERHEATING MOTOR!" "INVERTER ERROR!"
"INVERTER SERIAL BUS ERROR!"
"TEMPERATURE SENSOR ERROR"
"PRESSURE CONTROL FAILURE!"
"OPENING COVER in RUN!"
"SPEED METER ERROR"
"I2C BUS ERROR"
"OVERHEATING CENTRIFUGE!"
"ROTOR OVERSPEED!"
"COVER LOCK MALFUNCTION!"

12.2 Emergency cover release

	EMERGENCY COVER RELEASE <p>Attention! The cover may be opened in emergency only when the rotor is at rest. Before emergency opening the cover, switch off the mains power switch and disconnect the power cord. Wait 10 min and/or looking through the sight glass, make sure that the rotor is not rotating.</p> <p>To do this, insert the key for emergency opening of the cover (catalog number 17162) into the hole on the right side of the housing, and then push it until the lock is released and the cover is opened.</p> <p>The emergency opening of the cover can be used e.g., in the event of a power failure, failure of the control panel, etc.</p>
---	--

13 Guarantee

Manufacturer grants to the buyer the guarantee on conditions specified in the Guarantee Certificate. Buyer forfeits the right to guarantee repair when using the device inconsistently with the User manual provisions, when damage results from the User's fault.

Repairs should be carried out in authorized service workshops, granted with the MPW Certificate.

The centrifuge shall be sent to repair after decontaminating disinfections. Information about authorized service workshops could be obtained from the Manufacturer.



- Guarantee period amounts to 24 months (unless otherwise specified in the purchase documents).
- Guarantee conditions are described in guaranteed card.
- The service life of the centrifuge specified by the manufacturer amounts to 10 years.
- After 24 months from the start of the warranty period (date of purchase), a technical inspection of the centrifuge should be carried out (validation) by an authorized service of the manufacturer. Subsequent inspections should be carried out at annual intervals.
- Maximum period of storage of not used centrifuge amounts to 1 year. After this period, a service authorized by manufacturer should carry out technical inspection of the centrifuge.
- Manufacturer reserves the right to make technical changes in manufactured products.

14 Transport and storage



CAUTION! Due to the heavy weight of the device, lifting and carrying it may cause injury to the spine.

- Store the device only in a closed and dry room.
- Remove rotor from centrifuge before transport.
- Lift and carry with the adequate number of people.
- Use transport equipment.
- Use the original packaging and transport protection for transport.

14.1 Transport and storage conditions.

	Storage (in the package)	Storage (without the package)	Transport
Temperature	-25 ÷ +55 °C	-5 ÷ +45 °C	-25 ÷ +60 °C (general) -20 ÷ +55 °C (air)
Relative humidity	10 ÷ 75 %	10 ÷ 75 %	10 ÷ 75 %
Pressure	70 ÷ 106 kPa	70 ÷ 106 kPa	30 ÷ 106 kPa

15 Disposal



- Dispose of the device in accordance with the applicable legal regulations in the country of use.
- In the countries of the European Community, the disposal of electrical equipment is regulated under the EU Directive 2012/19/EU on waste electrical and electronic equipment (WEEE). According to these regulations, centrifuges may not be collected together with municipal or household waste.
- Disposal regulations in individual EU countries may differ. In case of doubt, please contact the supplier of the device.

16 List of changes in the manual

<i>Rev.</i>	<i>Release date</i>	<i>Description of changes</i>
19	03.04.2023	Addition of markings used in the manual and on the device. Update of nameplate, CE declaration and equipment lists. Updating records regarding the intended use and disposal of the product. Removal of the RTC function.
20	16.06.2023	Updating of the description in the technical data table. Updating the CE declaration of conformity, equipment list and nameplate.
21	20.09.2023	Removal of the USB communication function.
22	12.01.2024	Updated "Installation" chapter, equipment list and name plate.
23	08.01.2025	Updated chapters 1, 4, 5, 10 and 19. Restoration of Date/Time (RTC) function on selected units.

17 Manufacturer's info



"MPW MED. INSTRUMENTS" SPÓŁDZIELNIA PRACY
Boremlowska 46 Street
04-347 Warsaw
tel. (+48) 22 610 56 67 (sales department - POLAND)
(+48) 22 879 70 46 (sales department - outside POLAND)
(+48) 22 610 81 07 (service)
fax: (+48) 22 610 55 36
e-mail: mpw@mpw.pl
website: www.mpw.pl

000042924 - number of entries in the Waste Database

PL/CA01-01782 - identification number given by Office for Registration of Medicinal Products, Medical Devices and Biocidal Products.

18 Distributor's info

DISTRIBUTOR:

19 Annexes

A. Wyposażenie dodatkowe/Optional accessories**MPW-352/R/RH****WIRNIK / ROTOR**PARAMETRY/PARAMETERS (RCF [x g], Rmax [mm], α [$^{\circ}$])**POJEMNIK/BUCKET****WKŁADKA / ADAPTER**

[liczba próbówek na wirnik/tubes per rotor] PROBÓWKA / TUBE

11199RPM 18000 RCF 24270 Rmax 67 α 45**bez pojemnika/without bucket****bez wkładki/without adapter**

[12] * 2-1,5 ml próbówka (10,8x41,8 mm), Eppendorf®; [15011], 2 ml (10,8x41,8 mm); [15128], 1,5ml (10,8x40,5 mm)

14084[12] * 0,5 ml próbówka PCR (7,8 x 31 mm)
0,5 ml PCR tube (7,8 x 31 mm)**14126**[12] * 0,4 ml próbówka PCR (5,7 x 48,6 mm)
0,4 ml PCR tube (5,7 x 48,6 mm)**14133**[12] * 0,2 ml próbówka PCR (6 x 21,6 mm)
0,2 ml PCR tube (6 x 21,6 mm)**11210**RPM 5000 RCF 3997 Rmax 143 α 30**13080****14082**[24] * BD Vacutainer® (13 x 100 mm), (4-7 ml)
[24] * Greiner Vacuette® (13 x 100 mm), (3,5-6 ml)
[24] * Sarstedt S-Monovette® (11 x 92 mm), (4,5; 5 ml)
[24] * 6 ml próbówka z pokrywką (11,5 x 92 mm), Sarstedt®
6 ml tube with cap (11,5 x 92 mm), Sarstedt®
[24] * 7 ml próbówka szklana (12 x 100 mm)
7 ml glass tube (12 x 100 mm)
RCF max.=3000 RPM max.=4332**bez wkładki/without adapter**[24] 15046 14 ml próbówka z pokrywką (16,8 x 113,7 mm), Sarstedt®
14 ml tube with cap (16,8 x 113,7 mm), Sarstedt®[24] 15053 10 ml próbówka z pokrywką (16 x 106 mm)
10 ml tube with cap (16 x 106 mm)[24] * 15 ml próbówka z dnem stożkowym z zakrętką (17 x 120 mm), Falcon®; [15050], 15ml (17 x 120 mm)
15 ml tube, conical bottom, with cap (17 x 120 mm), Falcon®; [15050] 15ml Sarstedt®(17 x 120[24] * BD Vacutainer® (16 x 100 mm), (2,5-11 ml)
[24] * Greiner Vacuette® (16 x 100 mm), (7-9 ml)
[24] * Sarstedt S-Monovette® (15 x 92 mm), (7,5; 8,2; 8,5 ml)
[24] * Sarstedt S-Monovette® (16 x 92 mm), (9; 10 ml)
[24] * 15 ml Thermo Nalgene® (16 x 113 mm)
15 ml Thermo Nalgene® (16 x 113 mm)
[24] * 10 ml próbówka szklana (16 x 100 mm)
10 ml glass tube (16 x 100 mm)
RCF max.=3000 RPM max.=4332**14082+14815**[24] * 5 ml próbówka szklana (12 x 75 mm)
5 ml glass tube (12 x 75 mm)
RCF max.=3000 RPM max.=4509**14082+14815 Rmax 132 RCF 3689**[24] * BD Vacutainer® (13 x 75 mm), (1,6-5,3 ml)
[24] * Greiner Vacuette® (13 x 75 mm), (1-4,5 ml)
[24] * Sarstedt S-Monovette® (11 x 66 mm), (1,6; 2; 2,7; 3; 3,1 ml)
[24] * Sarstedt S-Monovette® (13 x 65 mm), (2,6; 2,9; 3,4; 3,8 ml)
[24] * Sarstedt S-Monovette® (13 x 75 mm), (2,7; 3; 4,3 ml)**14815 Rmax 132 RCF 3689**[24] 15121 10 ml próbówka z dnem okrągłym i pokrywką (17 x 70 mm)
10 ml tube, round bottom, with cap (17 x 70 mm)
[24] * Sarstedt S-Monovette® (15 x 75 mm), (4; 4,3; 5,5 ml)* próbówka niedostępna w ofercie MPW lub dostępny odpowiednik (np.: [15050]), patrz kolumna z prawej
tube is not offered by MPW or equivalent is available (e.g. [15050]), see column on the right

A. Wyposażenie dodatkowe/Optional accessories

MPW-352/R/RH

[24] * 10 ml Thermo Nalgene® Oak Ridge (16 x 81,5 mm)

11211

RPM 5500 RCF 4498 Rmax 133 4 30

13276

bez wkładki/without adapter

[10] 15051 50 ml Thermo Nalgene® Oak Ridge (28,8 x 106,7 mm)

50 ml Thermo Nalgene® Oak Ridge (28,8 x 106,7 mm)

[10] * 50 ml probówka z dnem stożkowym z zakrętką (30 x 117 mm), Falcon®; [15052] 50ml (30 x 117mm)

50 ml tube, conical bottom, with cap (30 x 117 mm), Falcon®; [15052] 50ml Sarstedt® (30 x 117

[10] * 50 ml probówka z dnem stożkowym bez rantu (30 x 115 mm), Greiner®

50 ml tube, conical bottom, without skirt (30 x 115 mm), Greiner®

[10] * 50 ml probówka Advanced Oak Ridge (29x102 mm), Herolab® nr 25 32 11

50 ml tube, Advanced Oak Ridge (29 x 102 mm), Herolab® no. 25 32 11

14035

[10] 15046 14 ml probówka z pokrywką (16,8 x 113,7 mm), Sarstedt®

14 ml tube with cap (16,8 x 113,7 mm), Sarstedt®

[10] 15053 10 ml probówka z pokrywką (16 x 106 mm)

10 ml tube with cap (16 x 106 mm)

[10] * 15 ml Thermo Nalgene® (16 x 113 mm)

15 ml Thermo Nalgene® (16 x 113 mm)

[10] * 10 ml probówka szklana (16 x 100 mm)

10 ml glass tube (16 x 100 mm)

RCF max.=3000 RPM max.=4492

14036

[10] * BD Vacutainer® (13 x 100 mm), (4-7 ml)

[10] * Greiner Vacuette® (13 x 100 mm), (3,5-6 ml)

[10] * 7 ml probówka szklana (12 x 100 mm)

7 ml glass tube (12 x 100 mm)

RCF max.=3000 RPM max.=4492

[10] * 6 ml probówka z pokrywką (11,5 x 92 mm), Sarstedt®

6 ml tube with cap (11,5 x 92 mm), Sarstedt®

14043

[10] * Greiner Vacuette® (13 x 75 mm), (1-4,5 ml)

[10] * Sarstedt S-Monovette® (13 x 75 mm), (2,7; 3; 4,3 ml)

[10] * Sarstedt S-Monovette® (13 x 90 mm), (4,9; 5,6 ml)

[10] * 5 ml probówka szklana (12 x 75 mm)

5 ml glass tube (12 x 75 mm)

RCF max.=3000 RPM max.=4492

[10] * 5 ml probówka z korkiem (12 x 85 mm), Sarstedt®

5 ml tube with cap (12 x 85 mm), Sarstedt®

14071

[10] 15055 30 ml probówka z pokrywką (25,4 x 103,2 mm)

30 ml tube with cap (25,4 x 103,2 mm)

[10] * 28 ml Thermo Nalgene® Oak Ridge (25,4 x 101,8 mm)

[10] * 30 ml probówka z pokrywką (25,5 x 94 mm), Nalgene®

30 ml tube with cap (25,5 x 94 mm), Nalgene®

[10] * 30 ml Thermo Nalgene® Oak Ridge (25,5 x 94,3 mm)

30 ml Thermo Nalgene® Oak Ridge (25,5 x 94,3 mm)

14073

[10] 15046 14 ml probówka z pokrywką (16,8 x 113,7 mm), Sarstedt®

14 ml tube with cap (16,8 x 113,7 mm), Sarstedt®

[10] 15053 10 ml probówka z pokrywką (16 x 106 mm)

10 ml tube with cap (16 x 106 mm)

[10] * Greiner Vacuette® (16 x 100 mm), (7-9 ml)

[10] * Sarstedt S-Monovette® (15 x 92 mm), (7,5; 8,2; 8,5 ml)

[10] * BD Vacutainer® (16 x 100 mm), (2,5-11 ml)

[10] * Sarstedt S-Monovette® (16 x 92 mm), (9; 10 ml)

[10] * 10 ml probówka szklana (16 x 100 mm)

10 ml glass tube (16 x 100 mm)

RCF max.=3000 RPM max.=4492

14089

[10] * 15 ml probówka z dnem stożkowym z zakrętką (17 x 120 mm), Falcon®; [15050], 15ml (17 x 120 mm)

15 ml tube, conical bottom, with cap (17 x 120 mm), Falcon®; [15050] 15ml Sarstedt®(17 x 120

14248

[10] 15055 30 ml probówka z pokrywką (25,4 x 103,2 mm)

30 ml tube with cap (25,4 x 103,2 mm)

14089+14868

[10] * 5 ml probówka z korkiem wciskanym (17 x 54,2 mm), Eppendorf®

5 ml tube with snap cap (17 x 54,2 mm), Eppendorf®

A. Wyposażenie dodatkowe/Optional accessories

MPW-352/R/RH

- [10] * 5 ml probówka z korkiem zakręcanym (17 x 66 mm), Eppendorf®
5 ml tube with screw cap (17 x 66 mm), Eppendorf®

13278+17151

bez wkładki/without adapter

- [10] 15051 50 ml Thermo Nalgene® Oak Ridge (28,8 x 106,7 mm)
50 ml Thermo Nalgene® Oak Ridge (28,8 x 106,7 mm)
- [10] * 50 ml probówka z dnem stożkowym z zakrętką (30 x 117 mm), Falcon®; [15052] 50ml (30 x 117mm)
50 ml tube, conical bottom, with cap (30 x 117 mm), Falcon®; [15052] 50ml Sarstedt® (30 x 117 mm)
- [10] * 50 ml probówka z dnem stożkowym bez rantu (30 x 115 mm), Greiner®
50 ml tube, conical bottom, without skirt (30 x 115 mm), Greiner®
- [10] * 50 ml probówka Advanced Oak Ridge (29x102 mm), Herolab® nr 25 32 11
50 ml tube, Advanced Oak Ridge (29 x 102 mm), Herolab® no. 25 32 11

14035

- [10] 15046 14 ml probówka z pokrywką (16,8 x 113,7 mm), Sarstedt®
14 ml tube with cap (16,8 x 113,7 mm), Sarstedt®
- [10] 15053 10 ml probówka z pokrywką (16 x 106 mm)
10 ml tube with cap (16 x 106 mm)
- [10] * 15 ml Thermo Nalgene® (16 x 113 mm)
15 ml Thermo Nalgene® (16 x 113 mm)
- [10] * 10 ml probówka szklana (16 x 100 mm)
10 ml glass tube (16 x 100 mm)
RCF max.=3000 RPM max.=4492

14036

- [10] * 7 ml probówka szklana (12 x 100 mm)
7 ml glass tube (12 x 100 mm)
RCF max.=3000 RPM max.=4492
- [10] * 6 ml probówka z pokrywką (11,5 x 92 mm), Sarstedt®
6 ml tube with cap (11,5 x 92 mm), Sarstedt®

14043

- [10] * Greiner Vacuette® (13 x 75 mm), (1-4,5 ml)
- [10] * 5 ml probówka szklana (12 x 75 mm)
5 ml glass tube (12 x 75 mm)
RCF max.=3000 RPM max.=4492
- [10] * 5 ml probówka z korkiem (12 x 85 mm), Sarstedt®
5 ml tube with cap (12 x 85 mm), Sarstedt®

14071

- [10] 15055 30 ml probówka z pokrywką (25,4 x 103,2 mm)
30 ml tube with cap (25,4 x 103,2 mm)
- [10] * 28 ml Thermo Nalgene® Oak Ridge (25,4 x 101,8 mm)
- [10] * 30 ml probówka z pokrywką (25,5 x 94 mm), Nalgene®
30 ml tube with cap (25,5 x 94 mm), Nalgene®
- [10] * 30 ml Thermo Nalgene® Oak Ridge (25,5 x 94,3 mm)
30 ml Thermo Nalgene® Oak Ridge (25,5 x 94,3 mm)

14073

- [10] 15046 14 ml probówka z pokrywką (16,8 x 113,7 mm), Sarstedt®
14 ml tube with cap (16,8 x 113,7 mm), Sarstedt®
- [10] 15053 10 ml probówka z pokrywką (16 x 106 mm)
10 ml tube with cap (16 x 106 mm)
- [10] * Greiner Vacuette® (16 x 100 mm), (7-9 ml)
- [10] * Sarstedt S-Monovette® (15 x 92 mm), (7,5; 8,2; 8,5 ml)
- [10] * BD Vacutainer® (16 x 100 mm), (2,5-11 ml)
- [10] * Sarstedt S-Monovette® (16 x 92 mm), (9; 10 ml)
- [10] * 10 ml probówka szklana (16 x 100 mm)
10 ml glass tube (16 x 100 mm)
RCF max.=3000 RPM max.=4492

14089

- [10] * 15 ml probówka z dnem stożkowym z zakrętką (17 x 120 mm), Falcon®; [15050], 15ml (17 x 120 mm)
15 ml tube, conical bottom, with cap (17 x 120 mm), Falcon®; [15050] 15ml Sarstedt®(17 x 120 mm)

14248

- [10] 15055 30 ml probówka z pokrywką (25,4 x 103,2 mm)
30 ml tube with cap (25,4 x 103,2 mm)

14089+14868

- [10] * 5 ml probówka z korkiem wciskanym (17 x 54,2 mm), Eppendorf®
5 ml tube with snap cap (17 x 54,2 mm), Eppendorf®

11213

RPM 5500 RCF 4227 Rmax 125 Δ 30

13276

bez wkładki/without adapter

A. Wyposażenie dodatkowe/Optional accessories

MPW-352/R/RH

[8] 15051	50 ml Thermo Nalgene® Oak Ridge (28,8 x 106,7 mm) 50 ml Thermo Nalgene® Oak Ridge (28,8 x 106,7 mm)
[8] *	50 ml probówka z dnem stożkowym z zakrętką (30 x 117 mm), Falcon®; [15052] 50ml (30 x 117mm) 50 ml tube, conical bottom, with cap (30 x 117 mm), Falcon®; [15052] 50ml Sarstedt® (30 x 117 mm)
[8] *	50 ml probówka z dnem stożkowym bez rantu (30 x 115 mm), Greiner® 50 ml tube, conical bottom, without skirt (30 x 115 mm), Greiner®
[8] *	50 ml probówka Advanced Oak Ridge (29x102 mm), Herolab® nr 25 32 11 50 ml tube, Advanced Oak Ridge (29 x 102 mm), Herolab® no. 25 32 11
	14035
[8] 15046	14 ml probówka z pokrywką (16,8 x 113,7 mm), Sarstedt® 14 ml tube with cap (16,8 x 113,7 mm), Sarstedt®
[8] 15053	10 ml probówka z pokrywką (16 x 106 mm) 10 ml tube with cap (16 x 106 mm)
[8] *	15 ml Thermo Nalgene® (16 x 113 mm) 15 ml Thermo Nalgene® (16 x 113 mm)
[8] *	10 ml probówka szklana (16 x 100 mm) 10 ml glass tube (16 x 100 mm) RCF max.=3000 RPM max.=4633
	14036
[8] *	BD Vacutainer® (13 x 100 mm), (4-7 ml)
[8] *	Greiner Vacuette® (13 x 100 mm), (3,5-6 ml)
[8] *	7 ml probówka szklana (12 x 100 mm) 7 ml glass tube (12 x 100 mm) RCF max.=3000 RPM max.=4633
[8] *	6 ml probówka z pokrywką (11,5 x 92 mm), Sarstedt® 6 ml tube with cap (11,5 x 92 mm), Sarstedt®
	14043
[8] *	Greiner Vacuette® (13 x 75 mm), (1-4,5 ml)
[8] *	Sarstedt S-Monovette® (13 x 75 mm), (2,7; 3; 4,3 ml)
[8] *	Sarstedt S-Monovette® (13 x 90 mm), (4,9; 5,6 ml)
[8] *	5 ml probówka szklana (12 x 75 mm) 5 ml glass tube (12 x 75 mm) RCF max.=3000 RPM max.=4633
[8] *	5 ml probówka z korkiem (12 x 85 mm), Sarstedt® 5 ml tube with cap (12 x 85 mm), Sarstedt®
	14071
[8] 15055	30 ml probówka z pokrywką (25,4 x 103,2 mm) 30 ml tube with cap (25,4 x 103,2 mm)
[8] *	28 ml Thermo Nalgene® Oak Ridge (25,4 x 101,8 mm)
[8] *	30 ml probówka z pokrywką (25,5 x 94 mm), Nalgene® 30 ml tube with cap (25,5 x 94 mm), Nalgene®
[8] *	30 ml Thermo Nalgene® Oak Ridge (25,5 x 94,3 mm) 30 ml Thermo Nalgene® Oak Ridge (25,5 x 94,3 mm)
	14073
[8] 15046	14 ml probówka z pokrywką (16,8 x 113,7 mm), Sarstedt® 14 ml tube with cap (16,8 x 113,7 mm), Sarstedt®
[8] 15053	10 ml probówka z pokrywką (16 x 106 mm) 10 ml tube with cap (16 x 106 mm)
[8] *	BD Vacutainer® (16 x 100 mm), (2,5-11 ml)
[8] *	Greiner Vacuette® (16 x 100 mm), (7-9 ml)
[8] *	Sarstedt S-Monovette® (15 x 92 mm), (7,5; 8,2; 8,5 ml)
[8] *	Sarstedt S-Monovette® (16 x 92 mm), (9; 10 ml)
[8] *	10 ml probówka szklana (16 x 100 mm) 10 ml glass tube (16 x 100 mm) RCF max.=3000 RPM max.=4633
	14089
[8] *	15 ml probówka z dnem stożkowym z zakrętką (17 x 120 mm), Falcon®; [15050], 15ml (17 x 120 mm) 15 ml tube, conical bottom, with cap (17 x 120 mm), Falcon®; [15050] 15ml Sarstedt®(17 x 120 mm)
	14248
[8] 15055	30 ml probówka z pokrywką (25,4 x 103,2 mm) 30 ml tube with cap (25,4 x 103,2 mm)
	14089+14868
[8] *	5 ml probówka z korkiem wciskanym (17 x 54,2 mm), Eppendorf® 5 ml tube with snap cap (17 x 54,2 mm), Eppendorf®
[8] *	5 ml probówka z korkiem zakręcanym (17 x 66 mm), Eppendorf® 5 ml tube with screw cap (17 x 66 mm), Eppendorf®
	13278+17151
	bez wkładki/without adapter
[8] 15051	50 ml Thermo Nalgene® Oak Ridge (28,8 x 106,7 mm) 50 ml Thermo Nalgene® Oak Ridge (28,8 x 106,7 mm)

* probówka niedostępna w ofercie MPW lub dostępny odpowiednik (np.[15050]), patrz kolumna z prawej
tube is not offered by MPW or equivalent is available (e.g. [15050]), see column on the right

A. Wyposażenie dodatkowe/Optional accessories

MPW-352/R/RH

[8] *	50 ml probówka z dnem stożkowym z zakrętką (30 x 117 mm), Falcon®; [15052] 50ml (30 x 117mm) 50 ml tube, conical bottom, with cap (30 x 117 mm), Falcon®; [15052] 50ml Sarstedt® (30 x 117
[8] *	50 ml probówka z dnem stożkowym bez rantu (30 x 115 mm), Greiner® 50 ml tube, conical bottom, without skirt (30 x 115 mm), Greiner®
[8] *	50 ml probówka Advanced Oak Ridge (29x102 mm), Herolab® nr 25 32 11 50 ml tube, Advanced Oak Ridge (29 x 102 mm), Herolab® no. 25 32 11
	14035
[8] 15046	14 ml probówka z pokrywką (16,8 x 113,7 mm), Sarstedt® 14 ml tube with cap (16,8 x 113,7 mm), Sarstedt®
[8] 15053	10 ml probówka z pokrywką (16 x 106 mm) 10 ml tube with cap (16 x 106 mm)
[8] *	15 ml Thermo Nalgene® (16 x 113 mm) 15 ml Thermo Nalgene® (16 x 113 mm)
[8] *	10 ml probówka szklana (16 x 100 mm) 10 ml glass tube (16 x 100 mm) RCF max.=3000 RPM max.=4633
	14036
[8] *	7 ml probówka szklana (12 x 100 mm) 7 ml glass tube (12 x 100 mm) RCF max.=3000 RPM max.=4633
[8] *	6 ml probówka z pokrywką (11,5 x 92 mm), Sarstedt® 6 ml tube with cap (11,5 x 92 mm), Sarstedt®
	14043
[8] *	Greiner Vacuette® (13 x 75 mm), (1-4,5 ml)
[8] *	5 ml probówka szklana (12 x 75 mm) 5 ml glass tube (12 x 75 mm) RCF max.=3000 RPM max.=4633
[8] *	5 ml probówka z korkiem (12 x 85 mm), Sarstedt® 5 ml tube with cap (12 x 85 mm), Sarstedt®
	14071
[8] 15055	30 ml probówka z pokrywką (25,4 x 103,2 mm) 30 ml tube with cap (25,4 x 103,2 mm)
[8] *	28 ml Thermo Nalgene® Oak Ridge (25,4 x 101,8 mm)
[8] *	30 ml probówka z pokrywką (25,5 x 94 mm), Nalgene® 30 ml tube with cap (25,5 x 94 mm), Nalgene®
[8] *	30 ml Thermo Nalgene® Oak Ridge (25,5 x 94,3 mm) 30 ml Thermo Nalgene® Oak Ridge (25,5 x 94,3 mm)
	14073
[8] 15046	14 ml probówka z pokrywką (16,8 x 113,7 mm), Sarstedt® 14 ml tube with cap (16,8 x 113,7 mm), Sarstedt®
[8] 15053	10 ml probówka z pokrywką (16 x 106 mm) 10 ml tube with cap (16 x 106 mm)
[8] *	BD Vacutainer® (16 x 100 mm), (2,5-11 ml)
[8] *	Greiner Vacuette® (16 x 100 mm), (7-9 ml)
[8] *	Sarstedt S-Monovette® (15 x 92 mm), (7,5; 8,2; 8,5 ml)
[8] *	Sarstedt S-Monovette® (16 x 92 mm), (9; 10 ml)
[8] *	10 ml probówka szklana (16 x 100 mm) 10 ml glass tube (16 x 100 mm) RCF max.=3000 RPM max.=4633
	14089
[8] *	15 ml probówka z dnem stożkowym z zakrętką (17 x 120 mm), Falcon®; [15050], 15ml (17 x 120 mm) 15 ml tube, conical bottom, with cap (17 x 120 mm), Falcon®; [15050] 15ml Sarstedt®(17 x 120
	14248
[8] 15055	30 ml probówka z pokrywką (25,4 x 103,2 mm) 30 ml tube with cap (25,4 x 103,2 mm)
	14089+14868
[8] *	5 ml probówka z korkiem wciskanym (17 x 54,2 mm), Eppendorf® 5 ml tube with snap cap (17 x 54,2 mm), Eppendorf®
11456	RPM 5000 RCF 4053 Rmax 145 4 30
	13080
	14082
[36] *	BD Vacutainer® (13 x 100 mm), (4-7 ml)
[36] *	Greiner Vacuette® (13 x 100 mm), (3,5-6 ml)
[36] *	Sarstedt S-Monovette® (11 x 92 mm), (4,5; 5 ml)
[36] *	6 ml probówka z pokrywką (11,5 x 92 mm), Sarstedt® 6 ml tube with cap (11,5 x 92 mm), Sarstedt®
[36] *	7 ml probówka szklana (12 x 100 mm) 7 ml glass tube (12 x 100 mm) RCF max.=3000 RPM max.=4302

* probówka niedostępna w ofercie MPW lub dostępny odpowiednik (np:[15050]), patrz kolumna z prawej
tube is not offered by MPW or equivalent is available (e.g. [15050]), see column on the right

A. Wyposażenie dodatkowe/Optional accessories

MPW-352/R/RH

bez wkładki/without adapter

[36] 15046	14 ml probówka z pokrywką (16,8 x 113,7 mm), Sarstedt® 14 ml tube with cap (16,8 x 113,7 mm), Sarstedt®
[36] 15053	10 ml probówka z pokrywką (16 x 106 mm) 10 ml tube with cap (16 x 106 mm)
[36] *	15 ml probówka z dnem stożkowym z zakrętką (17 x 120 mm), Falcon®; [15050], 15ml (17 x 120 mm) 15 ml tube, conical bottom, with cap (17 x 120 mm), Falcon®; [15050] 15ml Sarstedt®(17 x 120 mm)
[36] *	BD Vacutainer® (16 x 100 mm), (2,5-11 ml)
[36] *	Greiner Vacuette® (16 x 100 mm), (7-9 ml)
[36] *	Sarstedt S-Monovette® (15 x 92 mm), (7,5; 8,2; 8,5 ml)
[36] *	Sarstedt S-Monovette® (16 x 92 mm), (9; 10 ml)
[36] *	15 ml Thermo Nalgene® (16 x 113 mm) 15 ml Thermo Nalgene® (16 x 113 mm)
[36] *	10 ml probówka szklana (16 x 100 mm) 10 ml glass tube (16 x 100 mm) RCF max.=3000 RPM max.=4302
	14082+14815
[36] *	5 ml probówka szklana (12 x 75 mm) 5 ml glass tube (12 x 75 mm) RCF max.=3000 RPM max.=4509
	14082+14815 Rmax 132 RCF 3689
[36] *	BD Vacutainer® (13 x 75 mm), (1,6-5,3 ml)
[36] *	Greiner Vacuette® (13 x 75 mm), (1-4,5 ml)
[36] *	Sarstedt S-Monovette® (11 x 66 mm), (1,6; 2; 2,7; 3; 3,1 ml)
[36] *	Sarstedt S-Monovette® (13 x 65 mm), (2,6; 2,9; 3,4; 3,8 ml)
[36] *	Sarstedt S-Monovette® (13 x 75 mm), (2,7; 3; 4,3 ml)
	14815 Rmax 132 RCF 3689
[36] 15121	10 ml probówka z dnem okrągłym i pokrywką (17 x 70 mm) 10 ml tube, round bottom, with cap (17 x 70 mm)
[36] *	Sarstedt S-Monovette® (15 x 75 mm), (4; 4,3; 5,5 ml)
[36] *	10 ml Thermo Nalgene® Oak Ridge (16 x 81,5 mm)

11457

RPM 10000 RCF 10733 Rmax 96 4 30

bez pojemnika/without bucket

bez wkładki/without adapter

[6] *	50 ml probówka z dnem stożkowym z zakrętką (30 x 117 mm), Falcon®; [15052] 50ml (30 x 117mm) 50 ml tube, conical bottom, with cap (30 x 117 mm), Falcon®; [15052] 50ml Sarstedt® (30 x 117 mm)
[6] *	50 ml probówka z dnem stożkowym bez rantu (30 x 115 mm), Greiner® 50 ml tube, conical bottom, without skirt (30 x 115 mm), Greiner®
	14035
[6] 15046	14 ml probówka z pokrywką (16,8 x 113,7 mm), Sarstedt® 14 ml tube with cap (16,8 x 113,7 mm), Sarstedt®
[6] *	15 ml Thermo Nalgene® (16 x 113 mm) 15 ml Thermo Nalgene® (16 x 113 mm)
[6] *	10 ml probówka szklana (16 x 100 mm) 10 ml glass tube (16 x 100 mm) RCF max.=3000 RPM max.=5287
	14036
[6] *	7 ml probówka szklana (12 x 100 mm) 7 ml glass tube (12 x 100 mm) RCF max.=3000 RPM max.=5287
[6] *	6 ml probówka z pokrywką (11,5 x 92 mm), Sarstedt® 6 ml tube with cap (11,5 x 92 mm), Sarstedt®
	14043
[6] *	Greiner Vacuette® (13 x 75 mm), (1-4,5 ml)
[6] *	5 ml probówka szklana (12 x 75 mm) 5 ml glass tube (12 x 75 mm) RCF max.=3000 RPM max.=5287
[6] *	5 ml probówka z korkiem (12 x 85 mm), Sarstedt® 5 ml tube with cap (12 x 85 mm), Sarstedt®
	14071
[6] 15055	30 ml probówka z pokrywką (25,4 x 103,2 mm) 30 ml tube with cap (25,4 x 103,2 mm)
[6] *	28 ml Thermo Nalgene® Oak Ridge (25,4 x 101,8 mm)
[6] *	30 ml Thermo Nalgene® Oak Ridge (25,5 x 94,3 mm) 30 ml Thermo Nalgene® Oak Ridge (25,5 x 94,3 mm)
	14073
[6] 15046	14 ml probówka z pokrywką (16,8 x 113,7 mm), Sarstedt® 14 ml tube with cap (16,8 x 113,7 mm), Sarstedt®

* probówka niedostępna w ofercie MPW lub dostępny odpowiednik (np.: [15050]), patrz kolumna z prawej
tube is not offered by MPW or equivalent is available (e.g. [15050]), see column on the right

A. Wyposażenie dodatkowe/Optional accessories

MPW-352/R/RH

[6] 15053	10 ml probówka z pokrywką (16 x 106 mm) 10 ml tube with cap (16 x 106 mm)
[6] *	BD Vacutainer® (16 x 100 mm), (2,5-11 ml)
[6] *	Greiner Vacuette® (16 x 100 mm), (7-9 ml)
[6] *	10 ml probówka szklana (16 x 100 mm) 10 ml glass tube (16 x 100 mm) RCF max.=3000 RPM max.=5287
	14089
[6] *	15 ml probówka z dnem stożkowym z zakrętką (17 x 120 mm), Falcon®; [15050], 15ml (17 x 120 mm) 15 ml tube, conical bottom, with cap (17 x 120 mm), Falcon®; [15050] 15ml Sarstedt®(17 x 120 mm)
	14089+14868
[6] *	5 ml probówka z korkiem wciskanym (17 x 54,2 mm), Eppendorf® 5 ml tube with snap cap (17 x 54,2 mm), Eppendorf®
[6] *	5 ml probówka z korkiem zakręcanym (17 x 66 mm), Eppendorf® 5 ml tube with screw cap (17 x 66 mm), Eppendorf®

11458

RPM 15000 RCF 19621 Rmax 78 4 30

bez pojemnika/without bucket

bez wkładki/without adapter

[6] *	30 ml probówka z pokrywką (25,5 x 94 mm), Nalgene® 30 ml tube with cap (25,5 x 94 mm), Nalgene®
[6] *	30 ml Thermo Nalgene® Oak Ridge (25,5 x 94,3 mm) 30 ml Thermo Nalgene® Oak Ridge (25,5 x 94,3 mm)

11459

RPM 15000 RCF 21382 Rmax 85 4 30

bez pojemnika/without bucket

bez wkładki/without adapter

[12] 15121	10 ml probówka z dnem okrągłym i pokrywką (17 x 70 mm) 10 ml tube, round bottom, with cap (17 x 70 mm)
------------	---

11461

RPM 16000 RCF 23755 Rmax 83 4 45

bez pojemnika/without bucket

bez wkładki/without adapter

[24] *	2-1,5 ml probówka (10,8x41,8 mm), Eppendorf®; [15011], 2 ml (10,8x41,8 mm); [15128], 1,5ml (10,8x40,5 mm)
--------	---

14084

[24] *	0,5 ml probówka PCR (7,8 x 31 mm) 0,5 ml PCR tube (7,8 x 31 mm)
--------	--

14126

[24] *	0,4 ml probówka PCR (5,7 x 48,6 mm) 0,4 ml PCR tube (5,7 x 48,6 mm)
--------	--

14133

[24] *	0,2 ml probówka PCR (6 x 21,6 mm) 0,2 ml PCR tube (6 x 21,6 mm)
--------	--

11461

RPM 18000 RCF 30065 Rmax 83 4 45

bez pojemnika/without bucket

bez wkładki/without adapter

[24] *	2-1,5 ml probówka (10,8x41,8 mm), Eppendorf®; [15011], 2 ml (10,8x41,8 mm); [15128], 1,5ml (10,8x40,5 mm)
--------	---

14084

[24] *	0,5 ml probówka PCR (7,8 x 31 mm) 0,5 ml PCR tube (7,8 x 31 mm)
--------	--

14126

[24] *	0,4 ml probówka PCR (5,7 x 48,6 mm) 0,4 ml PCR tube (5,7 x 48,6 mm)
--------	--

14133

[24] *	0,2 ml probówka PCR (6 x 21,6 mm) 0,2 ml PCR tube (6 x 21,6 mm)
--------	--

11462

RPM 16000 RCF 23755 Rmax 83 4 45

bez pojemnika/without bucket

bez wkładki/without adapter

[36] *	2-1,5 ml probówka (10,8x41,8 mm), Eppendorf®; [15011], 2 ml (10,8x41,8 mm); [15128], 1,5ml (10,8x40,5 mm)
--------	---

14084

A. Wyposażenie dodatkowe/Optional accessories

MPW-352/R/RH

- [36] * 0,5 ml probówka PCR (7,8 x 31 mm)
0,5 ml PCR tube (7,8 x 31 mm)

14126

- [36] * 0,4 ml probówka PCR (5,7 x 48,6 mm)
0,4 ml PCR tube (5,7 x 48,6 mm)

14133

- [36] * 0,2 ml probówka PCR (6 x 21,6 mm)
0,2 ml PCR tube (6 x 21,6 mm)

11462

RPM 18000 RCF 30065 Rmax 83 4 45

bez pojemnika/without bucket

bez wkładki/without adapter

- [36] * 2-1,5 ml probówka (10,8x41,8 mm), Eppendorf®; [15011], 2 ml (10,8x41,8 mm); [15128], 1,5ml (10,8x40,5 mm)

14084

- [36] * 0,5 ml probówka PCR (7,8 x 31 mm)
0,5 ml PCR tube (7,8 x 31 mm)

14126

- [36] * 0,4 ml probówka PCR (5,7 x 48,6 mm)
0,4 ml PCR tube (5,7 x 48,6 mm)

14133

- [36] * 0,2 ml probówka PCR (6 x 21,6 mm)
0,2 ml PCR tube (6 x 21,6 mm)

11466

RPM 10000 RCF 10733 Rmax 96 4 29

bez pojemnika/without bucket

bez wkładki/without adapter

- [10] * 15 ml probówka z dnem stożkowym z zakrętką (17 x 120 mm), Falcon®; [15050], 15ml (17 x 120 mm)
15 ml tube, conical bottom, with cap (17 x 120 mm), Falcon®; [15050] 15ml Sarstedt®(17 x 120 mm)

14047

- [10] * 5 ml probówka z korkiem (12 x 85 mm), Sarstedt®
5 ml tube with cap (12 x 85 mm), Sarstedt®

14868

- [10] * 5 ml probówka z korkiem wciskanym (17 x 54,2 mm), Eppendorf®
5 ml tube with snap cap (17 x 54,2 mm), Eppendorf®

- [10] * 5 ml probówka z korkiem zatkaczanym (17 x 66 mm), Eppendorf®
5 ml tube with screw cap (17 x 66 mm), Eppendorf®

11467

RPM 12000 RCF 15133 Rmax 94 4 30

bez pojemnika/without bucket

bez wkładki/without adapter

- [12] 15046 14 ml probówka z pokrywką (16,8 x 113,7 mm), Sarstedt®
14 ml tube with cap (16,8 x 113,7 mm), Sarstedt®

- [12] 15053 10 ml probówka z pokrywką (16 x 106 mm)
10 ml tube with cap (16 x 106 mm)

- [12] * 15 ml Thermo Nalgene® (16 x 113 mm)
15 ml Thermo Nalgene® (16 x 113 mm)

11469

RPM 12000 RCF 14489 Rmax 90 4 30

bez pojemnika/without bucket

bez wkładki/without adapter

- [6] 15051 50 ml Thermo Nalgene® Oak Ridge (28,8 x 106,7 mm)
50 ml Thermo Nalgene® Oak Ridge (28,8 x 106,7 mm)

14035

- [6] 15046 14 ml probówka z pokrywką (16,8 x 113,7 mm), Sarstedt®
14 ml tube with cap (16,8 x 113,7 mm), Sarstedt®

- [6] 15053 10 ml probówka z pokrywką (16 x 106 mm)
10 ml tube with cap (16 x 106 mm)

14036

- [6] * 6 ml probówka z pokrywką (11,5 x 92 mm), Sarstedt®
6 ml tube with cap (11,5 x 92 mm), Sarstedt®

11501

RPM 5200 RCF 3960 Rmax 131 4 30

13080

14082

- [30] * BD Vacutainer® (13 x 100 mm), (4-7 ml)

A. Wyposażenie dodatkowe/Optional accessories

MPW-352/R/RH

[30] *	Greiner Vacuette® (13 x 100 mm), (3,5-6 ml)
[30] *	Sarstedt S-Monovette® (11 x 92 mm), (4,5; 5 ml)
[30] *	7 ml probówka szklana (12 x 100 mm) 7 ml glass tube (12 x 100 mm) RCF max.=3000 RPM max.=4526
[30] *	6 ml probówka z pokrywką (11,5 x 92 mm), Sarstedt® 6 ml tube with cap (11,5 x 92 mm), Sarstedt® bez wkładki/without adapter
[30] 15046	14 ml probówka z pokrywką (16,8 x 113,7 mm), Sarstedt® 14 ml tube with cap (16,8 x 113,7 mm), Sarstedt®
[30] 15053	10 ml probówka z pokrywką (16 x 106 mm) 10 ml tube with cap (16 x 106 mm)
[30] *	15 ml probówka z dnem stożkowym z zakrętką (17 x 120 mm), Falcon®; [15050], 15ml (17 x 120 mm) 15 ml tube, conical bottom, with cap (17 x 120 mm), Falcon®; [15050] 15ml Sarstedt®(17 x 120 mm)
[30] *	BD Vacutainer® (16 x 100 mm), (2,5-11 ml)
[30] *	Greiner Vacuette® (16 x 100 mm), (7-9 ml)
[30] *	Sarstedt S-Monovette® (15 x 92 mm), (7,5; 8,2; 8,5 ml)
[30] *	Sarstedt S-Monovette® (16 x 92 mm), (9; 10 ml)
[30] *	15 ml Thermo Nalgene® (16 x 113 mm) 15 ml Thermo Nalgene® (16 x 113 mm)
[30] *	10 ml probówka szklana (16 x 100 mm) 10 ml glass tube (16 x 100 mm) RCF max.=3000 RPM max.=4526
14082+14815	
[30] *	5 ml probówka szklana (12 x 75 mm) 5 ml glass tube (12 x 75 mm) RCF max.=3000 RPM max.=4729
14082+14815 Rmax 120 RCF 3628	
[30] *	BD Vacutainer® (13 x 75 mm), (1,6-5,3 ml)
[30] *	Greiner Vacuette® (13 x 75 mm), (1-4,5 ml)
[30] *	Sarstedt S-Monovette® (11 x 66 mm), (1,6; 2; 2,7; 3; 3,1 ml)
[30] *	Sarstedt S-Monovette® (13 x 65 mm), (2,6; 2,9; 3,4; 3,8 ml)
[30] *	Sarstedt S-Monovette® (13 x 75 mm), (2,7; 3; 4,3 ml)
14815 Rmax 120 RCF 3628	
[30] 15121	10 ml probówka z dnem okrągłym i pokrywką (17 x 70 mm) 10 ml tube, round bottom, with cap (17 x 70 mm)
[30] *	Sarstedt S-Monovette® (15 x 75 mm), (4; 4,3; 5,5 ml)
[30] *	10 ml Thermo Nalgene® Oak Ridge (16 x 81,5 mm)

11585

RPM 14000 RCF 20817 Rmax 95 4 45

bez pojemnika/without bucket

bez wkładki/without adapter

[12] *	8 x 0,2 ml probówki szeregowo PCR-strip (10,2 x 72,4 mm) 8 x 0,2 ml PCR strip (10,2 x 72,4 mm)
[96] *	0,2 ml probówka PCR (6 x 21,6 mm) 0,2 ml PCR tube (6 x 21,6 mm)
[12] *	8 x 0,2 ml probówki szeregowo PCR strip (7,3 x 77,2 mm) 8 x 0,2 ml PCR strip (7,3 x 77,2 mm)
[12] *	4 x 0,2 ml probówki szeregowo PCR-strip (10,2 x 37,2 mm) 4 x 0,2 ml PCR strip (10,2 x 37,2 mm)

11586

RPM 7000 RCF 6081 Rmax 111 4 35

13587

bez wkładki/without adapter

[6] *	85 ml Thermo Nalgene® Oak Ridge (38,2 x 105,7 mm) 85 ml Thermo Nalgene® Oak Ridge (38,2 x 105,7 mm)
14855	
[6] *	50 ml probówka z dnem stożkowym z zakrętką (30 x 117 mm), Falcon®; [15052] 50ml (30 x 117mm) 50 ml tube, conical bottom, with cap (30 x 117 mm), Falcon®; [15052] 50ml Sarstedt® (30 x 117 mm)
[6] *	50 ml probówka z dnem stożkowym bez rantu (30 x 115 mm), Greiner® 50 ml tube, conical bottom, without skirt (30 x 115 mm), Greiner®
14856	
[6] *	15 ml probówka z dnem stożkowym z zakrętką (17 x 120 mm), Falcon®; [15050], 15ml (17 x 120 mm) 15 ml tube, conical bottom, with cap (17 x 120 mm), Falcon®; [15050] 15ml Sarstedt®(17 x 120 mm)

11718

RPM 6300 RCF 5014 Rmax 113 4 30

13719

14024

A. Wyposażenie dodatkowe/Optional accessories

MPW-352/R/RH

[4] *	15 ml probówka z dnem stożkowym z zakrętką (17 x 120 mm), Falcon®; [15050], 15ml (17 x 120 mm) 15 ml tube, conical bottom, with cap (17 x 120 mm), Falcon®; [15050] 15ml Sarstedt®(17 x 120 14196
[4] 15040	100 ml probówka z pokrywką (45,2 x 103,7 mm) 100 ml tube with cap (45,2 x 103,7 mm) 14224
[4] 15055	30 ml probówka z pokrywką (25,4 x 103,2 mm) 30 ml tube with cap (25,4 x 103,2 mm)
[4] 15222	30 ml probówka z pokrywką (25 x 94mm), Sterilin® 30 ml tube with cap (25 x 94 mm), Sterilin®
[4] 15223	30 ml probówka z pokrywką (25 x 94 mm), Sterilin® 30 ml tube with cap (25 x 94 mm), Sterilin®
[4] *	30 ml Thermo Nalgene® Oak Ridge (25,5 x 94,3 mm) 30 ml Thermo Nalgene® Oak Ridge (25,5 x 94,3 mm) 14226
[4] *	50 ml probówka z dnem stożkowym z rantem (30 x 115 mm), Greiner® 50 ml tube, conical bottom, skirted (30 x 115 mm), Greiner® 14189+14188
[4] 15051	50 ml Thermo Nalgene® Oak Ridge (28,8 x 106,7 mm) 50 ml Thermo Nalgene® Oak Ridge (28,8 x 106,7 mm)
[4] *	50 ml probówka z dnem stożkowym z zakrętką (30 x 117 mm), Falcon®; [15052] 50ml (30 x 117mm) 50 ml tube, conical bottom, with cap (30 x 117 mm), Falcon®; [15052] 50ml Sarstedt® (30 x 117
[4] *	50 ml probówka z dnem stożkowym bez rantu (30 x 115 mm), Greiner® 50 ml tube, conical bottom, without skirt (30 x 115 mm), Greiner®
[4] *	50 ml probówka Advanced Oak Ridge (29x102 mm), Herolab® nr 25 32 11 50 ml tube, Advanced Oak Ridge (29 x 102 mm), Herolab® no. 25 32 11 14190+14188
[4] 15055	30 ml probówka z pokrywką (25,4 x 103,2 mm) 30 ml tube with cap (25,4 x 103,2 mm)
11740	RPM 5500 RCF 4058 Rmax 120 × 30

13080

14082

[12] *	BD Vacutainer® (13 x 100 mm), (4-7 ml)
[12] *	Greiner Vacuette® (13 x 100 mm), (3,5-6 ml)
[12] *	Sarstedt S-Monovette® (11 x 92 mm), (4,5; 5 ml)
[12] *	7 ml probówka szklana (12 x 100 mm) 7 ml glass tube (12 x 100 mm) RCF max.=3000 RPM max.=4729
[12] *	6 ml probówka z pokrywką (11,5 x 92 mm), Sarstedt® 6 ml tube with cap (11,5 x 92 mm), Sarstedt® bez wkładki/without adapter
[12] 15046	14 ml probówka z pokrywką (16,8 x 113,7 mm), Sarstedt® 14 ml tube with cap (16,8 x 113,7 mm), Sarstedt®
[12] 15053	10 ml probówka z pokrywką (16 x 106 mm) 10 ml tube with cap (16 x 106 mm)
[12] *	15 ml probówka z dnem stożkowym z zakrętką (17 x 120 mm), Falcon®; [15050], 15ml (17 x 120 mm) 15 ml tube, conical bottom, with cap (17 x 120 mm), Falcon®; [15050] 15ml Sarstedt®(17 x 120
[12] *	BD Vacutainer® (16 x 100 mm), (2,5-11 ml)
[12] *	Greiner Vacuette® (16 x 100 mm), (7-9 ml)
[12] *	Sarstedt S-Monovette® (15 x 92 mm), (7,5; 8,2; 8,5 ml)
[12] *	Sarstedt S-Monovette® (16 x 92 mm), (9; 10 ml)
[12] *	15 ml Thermo Nalgene® (16 x 113 mm) 15 ml Thermo Nalgene® (16 x 113 mm)
[12] *	10 ml probówka szklana (16 x 100 mm) 10 ml glass tube (16 x 100 mm) RCF max.=3000 RPM max.=4729 14082+14815
[12] *	5 ml probówka szklana (12 x 75 mm) 5 ml glass tube (12 x 75 mm) RCF max.=3000 RPM max.=5154 14082+14815 Rmax 101 RCF 3416
[12] *	BD Vacutainer® (13 x 75 mm), (1,6-5,3 ml)
[12] *	Greiner Vacuette® (13 x 75 mm), (1-4,5 ml)
[12] *	Sarstedt S-Monovette® (11 x 66 mm), (1,6; 2; 2,7; 3; 3,1 ml)
[12] *	Sarstedt S-Monovette® (13 x 65 mm), (2,6; 2,9; 3,4; 3,8 ml)
[12] *	Sarstedt S-Monovette® (13 x 75 mm), (2,7; 3; 4,3 ml)
	14815 Rmax 101 RCF 3416
[12] 15121	10 ml probówka z dnem okrągłym i pokrywką (17 x 70 mm) 10 ml tube, round bottom, with cap (17 x 70 mm)

* probówka niedostępna w ofercie MPW lub dostępny odpowiednik (np:[15050]), patrz kolumna z prawej
tube is not offered by MPW or equivalent is available (e.g. [15050]), see column on the right

A. Wyposażenie dodatkowe/Optional accessories

MPW-352/R/RH

- [12] * Sarstedt S-Monovette® (15 x 75 mm), (4; 4,3; 5,5 ml)
 [12] * 10 ml Thermo Nalgene® Oak Ridge (16 x 81,5 mm)

11743

RPM 5500 RCF 3889 Rmax 115 4 30

13329

bez wkładki/without adapter

- [12] 15055 30 ml probówka z pokrywką (25,4 x 103,2 mm)
 30 ml tube with cap (25,4 x 103,2 mm)
 [12] 15222 30 ml probówka z pokrywką (25 x 94mm), Sterilin®
 30 ml tube with cap (25 x 94 mm), Sterilin®
 [12] 15223 30 ml probówka z pokrywką (25 x 94 mm), Sterilin®
 30 ml tube with cap (25 x 94 mm), Sterilin®
 [12] * 30 ml probówka z pokrywką (25,5 x 94 mm), Nalgene®
 30 ml tube with cap (25,5 x 94 mm), Nalgene®

14256

- [12] 15046 14 ml probówka z pokrywką (16,8 x 113,7 mm), Sarstedt®
 14 ml tube with cap (16,8 x 113,7 mm), Sarstedt®
 [12] 15053 10 ml probówka z pokrywką (16 x 106 mm)
 10 ml tube with cap (16 x 106 mm)
 [12] * 15 ml Thermo Nalgene® (16 x 113 mm)
 15 ml Thermo Nalgene® (16 x 113 mm)
 [12] * 10 ml probówka szklana (16 x 100 mm)
 10 ml glass tube (16 x 100 mm)
 RCF max.=3000 RPM max.=4830

14255

- [12] * Sarstedt S-Monovette® (11 x 92 mm), (4,5; 5 ml)
 [12] * 7 ml probówka szklana (12 x 100 mm)
 7 ml glass tube (12 x 100 mm)
 RCF max.=3000 RPM max.=4830

11745

RPM 5000 RCF 3354 Rmax 120 4 30

13080

14082

- [24] * BD Vacutainer® (13 x 100 mm), (4-7 ml)
 [24] * Greiner Vacuette® (13 x 100 mm), (3,5-6 ml)
 [24] * Sarstedt S-Monovette® (11 x 92 mm), (4,5; 5 ml)
 [24] * 7 ml probówka szklana (12 x 100 mm)
 7 ml glass tube (12 x 100 mm)
 RCF max.=3000 RPM max.=4729

bez wkładki/without adapter

- [24] 15046 14 ml probówka z pokrywką (16,8 x 113,7 mm), Sarstedt®
 14 ml tube with cap (16,8 x 113,7 mm), Sarstedt®
 [24] 15053 10 ml probówka z pokrywką (16 x 106 mm)
 10 ml tube with cap (16 x 106 mm)
 [24] * 15 ml probówka z dnem stożkowym z zakrętką (17 x 120 mm), Falcon®; [15050], 15ml (17 x 120 mm)
 15 ml tube, conical bottom, with cap (17 x 120 mm), Falcon®; [15050] 15ml Sarstedt®(17 x 120 mm)
 [24] * BD Vacutainer® (16 x 100 mm), (2,5-11 ml)
 [24] * Greiner Vacuette® (16 x 100 mm), (7-9 ml)
 [24] * Sarstedt S-Monovette® (15 x 92 mm), (7,5; 8,2; 8,5 ml)
 [24] * Sarstedt S-Monovette® (16 x 92 mm), (9; 10 ml)
 [24] * 15 ml Thermo Nalgene® (16 x 113 mm)
 15 ml Thermo Nalgene® (16 x 113 mm)
 [24] * 10 ml probówka szklana (16 x 100 mm)
 10 ml glass tube (16 x 100 mm)
 RCF max.=3000 RPM max.=4729

14082+14815 Rmax 105 RCF 2935

- [24] * BD Vacutainer® (13 x 75 mm), (1,6-5,3 ml)
 [24] * Greiner Vacuette® (13 x 75 mm), (1-4,5 ml)
 [24] * Sarstedt S-Monovette® (11 x 66 mm), (1,6; 2; 2,7; 3; 3,1 ml)
 [24] * Sarstedt S-Monovette® (13 x 65 mm), (2,6; 2,9; 3,4; 3,8 ml)
 [24] * Sarstedt S-Monovette® (13 x 75 mm), (2,7; 3; 4,3 ml)
 [24] * 5 ml probówka szklana (12 x 75 mm)
 5 ml glass tube (12 x 75 mm)

14815 Rmax 105 RCF 2935

- [24] 15121 10 ml probówka z dnem okrągłym i pokrywką (17 x 70 mm)
 10 ml tube, round bottom, with cap (17 x 70 mm)
 [24] * Sarstedt S-Monovette® (15 x 75 mm), (4; 4,3; 5,5 ml)
 [24] * 10 ml Thermo Nalgene® Oak Ridge (16 x 81,5 mm)

A. Wyposażenie dodatkowe/Optional accessories

MPW-352/R/RH

11746

RPM 6000 RCF 4427 Rmax 110 Δ 30

13276

bez wkładki/without adapter

- [6] * 50 ml próbówka z dnem stożkowym z zakrętką (30 x 117 mm), Falcon®; [15052] 50ml (30 x 117mm)
50 ml tube, conical bottom, with cap (30 x 117 mm), Falcon®; [15052] 50ml Sarstedt® (30 x 117 mm)
- [6] * 50 ml próbówka z dnem stożkowym bez rantu (30 x 115 mm), Greiner®
50 ml tube, conical bottom, without skirt (30 x 115 mm), Greiner®
- [6] 15051 50 ml Thermo Nalgene® Oak Ridge (28,8 x 106,7 mm)
50 ml Thermo Nalgene® Oak Ridge (28,8 x 106,7 mm)
- [6] * 50 ml próbówka Advanced Oak Ridge (29x102 mm), Herolab® nr 25 32 11
50 ml tube, Advanced Oak Ridge (29 x 102 mm), Herolab® no. 25 32 11

14035

- [6] 15046 14 ml próbówka z pokrywką (16,8 x 113,7 mm), Sarstedt®
14 ml tube with cap (16,8 x 113,7 mm), Sarstedt®
- [6] 15053 10 ml próbówka z pokrywką (16 x 106 mm)
10 ml tube with cap (16 x 106 mm)
- [6] * 15 ml Thermo Nalgene® (16 x 113 mm)
15 ml Thermo Nalgene® (16 x 113 mm)
- [6] * 10 ml próbówka szklana (16 x 100 mm)
10 ml glass tube (16 x 100 mm)
RCF max.=3000 RPM max.=4939

14036

- [6] * BD Vacutainer® (13 x 100 mm), (4-7 ml)
- [6] * Greiner Vacvette® (13 x 100 mm), (3,5-6 ml)
- [6] * 7 ml próbówka szklana (12 x 100 mm)
7 ml glass tube (12 x 100 mm)
RCF max.=3000 RPM max.=4939
- [6] * 6 ml próbówka z pokrywką (11,5 x 92 mm), Sarstedt®
6 ml tube with cap (11,5 x 92 mm), Sarstedt®

14043

- [6] * Greiner Vacvette® (13 x 75 mm), (1-4,5 ml)
- [6] * Sarstedt S-Monovette® (13 x 75 mm), (2,7; 3; 4,3 ml)
- [6] * Sarstedt S-Monovette® (13 x 90 mm), (4,9; 5,6 ml)
- [6] * 5 ml próbówka z korkiem (12 x 85 mm), Sarstedt®
5 ml tube with cap (12 x 85 mm), Sarstedt®
- [6] * 5 ml próbówka szklana (12 x 75 mm)
5 ml glass tube (12 x 75 mm)
RCF max.=3000 RPM max.=4939

14071

- [6] 15055 30 ml próbówka z pokrywką (25,4 x 103,2 mm)
30 ml tube with cap (25,4 x 103,2 mm)
- [6] * 28 ml Thermo Nalgene® Oak Ridge (25,4 x 101,8 mm)
- [6] * 30 ml próbówka z pokrywką (25,5 x 94 mm), Nalgene®
30 ml tube with cap (25,5 x 94 mm), Nalgene®
- [6] * 30 ml Thermo Nalgene® Oak Ridge (25,5 x 94,3 mm)
30 ml Thermo Nalgene® Oak Ridge (25,5 x 94,3 mm)

14073

- [6] 15046 14 ml próbówka z pokrywką (16,8 x 113,7 mm), Sarstedt®
14 ml tube with cap (16,8 x 113,7 mm), Sarstedt®
- [6] 15053 10 ml próbówka z pokrywką (16 x 106 mm)
10 ml tube with cap (16 x 106 mm)
- [6] * BD Vacutainer® (16 x 100 mm), (2,5-11 ml)
- [6] * Greiner Vacvette® (16 x 100 mm), (7-9 ml)
- [6] * Sarstedt S-Monovette® (15 x 92 mm), (7,5; 8,2; 8,5 ml)
- [6] * Sarstedt S-Monovette® (16 x 92 mm), (9; 10 ml)
- [6] * 10 ml próbówka szklana (16 x 100 mm)
10 ml glass tube (16 x 100 mm)
RCF max.=3000 RPM max.=4939

14089

- [6] * 15 ml próbówka z dnem stożkowym z zakrętką (17 x 120 mm), Falcon®; [15050], 15ml (17 x 120 mm)
15 ml tube, conical bottom, with cap (17 x 120 mm), Falcon®; [15050] 15ml Sarstedt®(17 x 120 mm)

14248

- [6] 15055 30 ml próbówka z pokrywką (25,4 x 103,2 mm)
30 ml tube with cap (25,4 x 103,2 mm)

14089+14868

- [6] * 5 ml próbówka z korkiem wciskanym (17 x 54,2 mm), Eppendorf®
5 ml tube with snap cap (17 x 54,2 mm), Eppendorf®
- [6] * 5 ml próbówka z korkiem zakręcanym (17 x 66 mm), Eppendorf®
5 ml tube with screw cap (17 x 66 mm), Eppendorf®

A. Wyposażenie dodatkowe/Optional accessories

MPW-352/R/RH

11760

RPM 13000 RCF 16060 Rmax 85 4 45

bez pojemnika/without bucket

bez wkładki/without adapter

[24] * 2-1,5 ml probówka (10,8x41,8 mm), Eppendorf®; [15011], 2 ml (10,8x41,8 mm); [15128], 1,5ml (10,8x40,5 mm)

[24] * 2 ml probówki z filtrem - spin columns (10,8 x 46 mm)
2 ml spin columns (with filter) (10,8 x 46 mm); [15011], 2 ml (10,8x41,8 mm); [15128], 1,5ml
14084

[24] * 0,5 ml probówka PCR (7,8 x 31 mm)
0,5 ml PCR tube (7,8 x 31 mm)

14126

[24] * 0,4 ml probówka PCR (5,7 x 48,6 mm)
0,4 ml PCR tube (5,7 x 48,6 mm)

14133

[24] * 0,2 ml probówka PCR (6 x 21,6 mm)
0,2 ml PCR tube (6 x 21,6 mm)

11760

RPM 15000 RCF 21382 Rmax 85 4 45

bez pojemnika/without bucket

bez wkładki/without adapter

[24] * 2-1,5 ml probówka (10,8x41,8 mm), Eppendorf®; [15011], 2 ml (10,8x41,8 mm); [15128], 1,5ml (10,8x40,5 mm)

[24] * 2 ml probówki z filtrem - spin columns (10,8 x 46 mm)
2 ml spin columns (with filter) (10,8 x 46 mm); [15011], 2 ml (10,8x41,8 mm); [15128], 1,5ml
14084

[24] * 0,5 ml probówka PCR (7,8 x 31 mm)
0,5 ml PCR tube (7,8 x 31 mm)

14126

[24] * 0,4 ml probówka PCR (5,7 x 48,6 mm)
0,4 ml PCR tube (5,7 x 48,6 mm)

14133

[24] * 0,2 ml probówka PCR (6 x 21,6 mm)
0,2 ml PCR tube (6 x 21,6 mm)

11944

RPM 15000 RCF 21382 Rmax 85 4 45

bez pojemnika/without bucket

bez wkładki/without adapter

[6] * 5 ml probówka z korkiem zakręcanym (17 x 66 mm), Eppendorf®
5 ml tube with screw cap (17 x 66 mm), Eppendorf®

[12] * 5 ml probówka z korkiem wciskanym (17 x 54,2 mm), Eppendorf®
5 ml tube with snap cap (17 x 54,2 mm), Eppendorf®

12285

RPM 4500 RCF 2604 Rmax 115 4 90

13286

bez wkładki/without adapter

[2] * płytka titracyjna DWP 96/2000µl (127,8x85,5x44,1 mm)
deepwell plate DWP 96/2000µl (127,8 x 85,5 x 44,1 mm)

[8] * płytka titracyjna MTP 28,8ml (86x128x15/17,5 mm)
microtiter plate MTP 28,8 ml (86 x 128 x 15/17,5 mm)

12300

RPM 13000 RCF 16816 Rmax 89 4 90

bez pojemnika/without bucket

bez wkładki/without adapter

[24] * 37 µl kapilara hematokrytowa (1,4 x 75 mm)
37 µl micro-hematocrit capillary tube (1,4 x 75 mm)

16164

bez wkładki/without adapter

[24] * 37 µl kapilara hematokrytowa (1,4 x 75 mm)
37 µl micro-hematocrit capillary tube (1,4 x 75 mm)

12352

RPM 4800 RCF 4405 Rmax 171 4 90

13352

14050

A. Wyposażenie dodatkowe/Optional accessories

MPW-352/R/RH

[16]	*	50 ml probówka z dnem stożkowym z zakrętką (30 x 117 mm), Falcon®; [15052] 50ml (30 x 117mm) 50 ml tube, conical bottom, with cap (30 x 117 mm), Falcon®; [15052] 50ml Sarstedt® (30 x 117
[16]	*	50 ml probówka z dnem stożkowym bez rantu (30 x 115 mm), Greiner® 50 ml tube, conical bottom, without skirt (30 x 115 mm), Greiner®
		14051
[12]	*	50 ml probówka z dnem stożkowym z zakrętką (30 x 117 mm), Falcon®; [15052] 50ml (30 x 117mm) 50 ml tube, conical bottom, with cap (30 x 117 mm), Falcon®; [15052] 50ml Sarstedt® (30 x 117
[12]	*	50 ml probówka z dnem stożkowym bez rantu (30 x 115 mm), Greiner® 50 ml tube, conical bottom, without skirt (30 x 115 mm), Greiner®
		14250+14017
[4]	*	250 ml butelka okrąglodenna (62 x 122 mm), Herolab® nr 25 34 43 250 ml round-bottom bottle (62 x 122 mm), Herolab® no. 25 34 43
		14250+14175
[4]	15175	250 ml butelka płaskodenna (62 x 122 mm), Herolab® nr 25 34 21 250 ml bottle, flat bottom (62 x 122 mm), Herolab® no. 25 34 21
[4]	15176	250 ml butelka płaskodenna (62 x 122 mm), Herolab® nr 25 34 01 250 ml bottle,flat bottom (62 x 122 mm), Herolab® no. 25 34 01
		14310
[4]	15040	100 ml probówka z pokrywką (45,2 x 103,7 mm) 100 ml tube with cap (45,2 x 103,7 mm)
[4]	*	100 ml probówka szklana (44 x 100 mm) 100 ml glass tube (44 x 100 mm) RCF max.=4000 RPM max.=4574
		14311
[8]	*	50 ml probówka z dnem stożkowym z rantem (30 x 115 mm), Greiner® 50 ml tube, conical bottom, skirted (30 x 115 mm), Greiner®
		14312
[12]	*	50 ml probówka szklana (35 x 100 mm) 50 ml glass tube (35 x 100 mm) RCF max.=4000 RPM max.=4574
		14313
[76]	*	BD Vacutainer® (13 x 75 mm), (1,6-5,3 ml)
[76]	*	BD Vacutainer® (13 x 100 mm), (4-7 ml)
[76]	*	Sarstedt S-Monovette® (11 x 66 mm), (1,6; 2; 2,7; 3; 3,1 ml)
[76]	*	Sarstedt S-Monovette® (11 x 92 mm), (4,5; 5 ml)
[76]	*	Greiner Vacuette® (13 x 100 mm), (3,5-6 ml)
[76]	*	5 ml probówka z korkiem (12 x 85 mm), Sarstedt® 5 ml tube with cap (12 x 85 mm), Sarstedt®
[76]	*	6 ml probówka z pokrywką (11,5 x 92 mm), Sarstedt® 6 ml tube with cap (11,5 x 92 mm), Sarstedt®
		14314
[76]	*	BD Vacutainer® (13 x 75 mm), (1,6-5,3 ml)
[76]	*	Sarstedt S-Monovette® (11 x 66 mm), (1,6; 2; 2,7; 3; 3,1 ml)
[76]	*	Greiner Vacuette® (13 x 75 mm), (1-4,5 ml)
		14315
[32]	*	15 ml probówka z dnem stożkowym z zakrętką (17 x 120 mm), Falcon®; [15050], 15ml (17 x 120 mm) 15 ml tube, conical bottom, with cap (17 x 120 mm), Falcon®; [15050] 15ml Sarstedt®(17 x 120
		14315+14324
[32]	*	5 ml probówka z korkiem wciskanym (17 x 54,2 mm), Eppendorf® 5 ml tube with snap cap (17 x 54,2 mm), Eppendorf®
[32]	*	5 ml probówka z korkiem zakręcanym (17 x 66 mm), Eppendorf® 5 ml tube with screw cap (17 x 66 mm), Eppendorf®
		14316
[60]	*	BD Vacutainer® (16 x 100 mm), (2,5-11 ml)
[60]	*	Greiner Vacuette® (16 x 100 mm), (7-9 ml)
[60]	15053	10 ml probówka z pokrywką (16 x 106 mm) 10 ml tube with cap (16 x 106 mm)
[60]	*	Sarstedt S-Monovette® (15 x 92 mm), (7,5; 8,2; 8,5 ml)
[60]	*	Sarstedt S-Monovette® (15 x 75 mm), (4; 4,3; 5,5 ml)
[60]	*	10 ml Thermo Nalgene® Oak Ridge (16 x 81,5 mm)
[60]	15046	14 ml probówka z pokrywką (16,8 x 113,7 mm), Sarstedt® 14 ml tube with cap (16,8 x 113,7 mm), Sarstedt®
[60]	*	10 ml probówka szklana (16 x 100 mm) 10 ml glass tube (16 x 100 mm) RCF max.=4000 RPM max.=4574
		14317
[28]	*	15 ml probówka z dnem stożkowym z zakrętką (17 x 120 mm), Falcon®; [15050], 15ml (17 x 120 mm) 15 ml tube, conical bottom, with cap (17 x 120 mm), Falcon®; [15050] 15ml Sarstedt®(17 x 120
		14317+14324
[28]	*	5 ml probówka z korkiem wciskanym (17 x 54,2 mm), Eppendorf® 5 ml tube with snap cap (17 x 54,2 mm), Eppendorf®

* probówka niedostępna w ofercie MPW lub dostępny odpowiednik (np:[15050]), patrz kolumna z prawej
tube is not offered by MPW or equivalent is available (e.g. [15050]), see column on the right

A. Wyposażenie dodatkowe/Optional accessories

MPW-352/R/RH

[28]	*	5 ml probówka z korkiem zakręcanym (17 x 66 mm), Eppendorf® 5 ml tube with screw cap (17 x 66 mm), Eppendorf®
		14318
[104]	*	Sarstedt S-Monovette® (11 x 92 mm), (4,5; 5 ml)
[104]	*	Sarstedt S-Monovette® (11 x 66 mm), (1,6; 2; 2,7; 3; 3,1 ml)
[104]	*	7 ml probówka szklana (12 x 100 mm) 7 ml glass tube (12 x 100 mm) RCF max.=4000 RPM max.=4574
[104]	*	5 ml probówka szklana (12 x 75 mm) 5 ml glass tube (12 x 75 mm) RCF max.=4000 RPM max.=4574
[104]	*	5 ml probówka z korkiem (12 x 85 mm), Sarstedt® 5 ml tube with cap (12 x 85 mm), Sarstedt®
[104]	*	6 ml probówka z pokrywką (11,5 x 92 mm), Sarstedt® 6 ml tube with cap (11,5 x 92 mm), Sarstedt®
		14319
[28]	15055	30 ml probówka z pokrywką (25,4 x 103,2 mm) 30 ml tube with cap (25,4 x 103,2 mm)
[28]	*	28 ml Thermo Nalgene® Oak Ridge (25,4 x 101,8 mm)
[12]	15222	30 ml probówka z pokrywką (25 x 94mm), Sterilin® 30 ml tube with cap (25 x 94 mm), Sterilin®
[12]	15223	30 ml probówka z pokrywką (25 x 94 mm), Sterilin® 30 ml tube with cap (25 x 94 mm), Sterilin®
[28]	*	30 ml probówka z pokrywką (25,5 x 94 mm), Nalgene® 30 ml tube with cap (25,5 x 94 mm), Nalgene®
[28]	*	30 ml Thermo Nalgene® Oak Ridge (25,5 x 94,3 mm) 30 ml Thermo Nalgene® Oak Ridge (25,5 x 94,3 mm)
[28]	*	25 ml probówka szklana (25 x 100 mm) 25 ml glass tube (25 x 100 mm) RCF max.=4000 RPM max.=4574
		14320
[48]	15046	14 ml probówka z pokrywką (16,8 x 113,7 mm), Sarstedt® 14 ml tube with cap (16,8 x 113,7 mm), Sarstedt®
[48]	15053	10 ml probówka z pokrywką (16 x 106 mm) 10 ml tube with cap (16 x 106 mm)
[48]	*	BD Vacutainer® (16 x 100 mm), (2,5-11 ml)
[48]	*	Greiner Vacuette® (16 x 100 mm), (7-9 ml)
[48]	*	Sarstedt S-Monovette® (15 x 92 mm), (7,5; 8,2; 8,5 ml)
[48]	*	Sarstedt S-Monovette® (16 x 92 mm), (9; 10 ml)
[48]	15121	10 ml probówka z dnem okrągłym i pokrywką (17 x 70 mm) 10 ml tube, round bottom, with cap (17 x 70 mm)
[48]	*	Sarstedt S-Monovette® (15 x 75 mm), (4; 4,3; 5,5 ml)
[48]	*	10 ml Thermo Nalgene® Oak Ridge (16 x 81,5 mm)
[48]	*	15 ml Thermo Nalgene® (16 x 113 mm) 15 ml Thermo Nalgene® (16 x 113 mm)
[48]	*	13 ml probówka (16x100mm), Sarstedt® nr 62.515.006 13 ml tube (16 x 100 mm), Sarstedt® no. 62.515.006
[48]	*	10 ml probówka szklana (16 x 100 mm) 10 ml glass tube (16 x 100 mm) RCF max.=4000 RPM max.=4574
		14321
[16]	15051	50 ml Thermo Nalgene® Oak Ridge (28,8 x 106,7 mm) 50 ml Thermo Nalgene® Oak Ridge (28,8 x 106,7 mm)
[16]	*	50 ml probówka Advanced Oak Ridge (29x102 mm), Herolab® nr 25 32 11 50 ml tube, Advanced Oak Ridge (29 x 102 mm), Herolab® no. 25 32 11
		14322
[72]	*	2-1,5 ml probówka (10,8x41,8 mm), Eppendorf®; [15011], 2 ml (10,8x41,8 mm); [15128], 1,5ml (10,8x40,5 mm)
		14323
[4]	15440	200 ml butelka płaskodenna (56 x 112 mm), Herolab® nr 25 33 73 200 ml bottle, flat bottom (56 x 112 mm), Herolab® no. 25 33 73
		14325
[68]	*	BD Vacutainer® (13 x 75 mm), (1,6-5,3 ml)
[68]	*	Sarstedt S-Monovette® (13 x 90 mm), (4,9; 5,6 ml)
[68]	*	Greiner Vacuette® (13 x 100 mm), (3,5-6 ml)
[68]	*	BD Vacutainer® (13 x 100 mm), (4-7 ml)
[68]	*	Greiner Vacuette® (13 x 75 mm), (1-4,5 ml)
[68]	*	Sarstedt S-Monovette® (13 x 75 mm), (2,7; 3; 4,3 ml)
[68]	*	Sarstedt S-Monovette® (11 x 66 mm), (1,6; 2; 2,7; 3; 3,1 ml)
[68]	*	Sarstedt S-Monovette® (11 x 92 mm), (4,5; 5 ml)
[68]	*	Sarstedt S-Monovette® (13 x 65 mm), (2,6; 2,9; 3,4; 3,8 ml)

* probówka niedostępna w ofercie MPW lub dostępny odpowiednik (np.[15050]), patrz kolumna z prawej
tube is not offered by MPW or equivalent is available (e.g. [15050]), see column on the right

A. Wyposażenie dodatkowe/Optional accessories

MPW-352/R/RH

[68] *	5 ml probówka z korkiem (12 x 85 mm), Sarstedt® 5 ml tube with cap (12 x 85 mm), Sarstedt®
[68] *	6 ml probówka z pokrywką (11,5 x 92 mm), Sarstedt® 6 ml tube with cap (11,5 x 92 mm), Sarstedt®
13353+17353	
14051	
[12] *	50 ml probówka z dnem stożkowym z zakrętką (30 x 117 mm), Falcon®; [15052] 50ml (30 x 117mm) 50 ml tube, conical bottom, with cap (30 x 117 mm), Falcon®; [15052] 50ml Sarstedt® (30 x 117 mm)
[12] *	50 ml probówka z dnem stożkowym bez rantu (30 x 115 mm), Greiner® 50 ml tube, conical bottom, without skirt (30 x 115 mm), Greiner®
14250+14017	
[4] *	250 ml butelka okrąglodenna (62 x 122 mm), Herolab® nr 25 34 43 250 ml round-bottom bottle (62 x 122 mm), Herolab® no. 25 34 43
14250+14175	
[4] 15175	250 ml butelka płaskodenna (62 x 122 mm), Herolab® nr 25 34 21 250 ml bottle, flat bottom (62 x 122 mm), Herolab® no. 25 34 21
[4] 15176	250 ml butelka płaskodenna (62 x 122 mm), Herolab® nr 25 34 01 250 ml bottle, flat bottom (62 x 122 mm), Herolab® no. 25 34 01
14310	
[4] 15040	100 ml probówka z pokrywką (45,2 x 103,7 mm) 100 ml tube with cap (45,2 x 103,7 mm)
[4] *	100 ml probówka szklana (44 x 100 mm) 100 ml glass tube (44 x 100 mm) RCF max.=4000 RPM max.=4574
14311	
[8] *	50 ml probówka z dnem stożkowym z rantem (30 x 115 mm), Greiner® 50 ml tube, conical bottom, skirted (30 x 115 mm), Greiner®
14312	
[12] *	50 ml probówka szklana (35 x 100 mm) 50 ml glass tube (35 x 100 mm) RCF max.=4000 RPM max.=4574
14313	
[76] *	BD Vacutainer® (13 x 75 mm), (1,6-5,3 ml)
[76] *	BD Vacutainer® (13 x 100 mm), (4-7 ml)
[76] *	Sarstedt S-Monovette® (11 x 66 mm), (1,6; 2; 2,7; 3; 3,1 ml)
[76] *	Sarstedt S-Monovette® (11 x 92 mm), (4,5; 5 ml)
[76] *	Greiner Vacuette® (13 x 100 mm), (3,5-6 ml)
[76] *	5 ml probówka z korkiem (12 x 85 mm), Sarstedt® 5 ml tube with cap (12 x 85 mm), Sarstedt®
[76] *	6 ml probówka z pokrywką (11,5 x 92 mm), Sarstedt® 6 ml tube with cap (11,5 x 92 mm), Sarstedt®
14314	
[76] *	BD Vacutainer® (13 x 75 mm), (1,6-5,3 ml)
[76] *	Sarstedt S-Monovette® (11 x 66 mm), (1,6; 2; 2,7; 3; 3,1 ml)
[76] *	Greiner Vacuette® (13 x 75 mm), (1-4,5 ml)
14315+14324	
[32] *	5 ml probówka z korkiem wciskanym (17 x 54,2 mm), Eppendorf® 5 ml tube with snap cap (17 x 54,2 mm), Eppendorf®
[32] *	5 ml probówka z korkiem zakręcanym (17 x 66 mm), Eppendorf® 5 ml tube with screw cap (17 x 66 mm), Eppendorf®
14316	
[60] *	BD Vacutainer® (16 x 100 mm), (2,5-11 ml)
[60] *	Greiner Vacuette® (16 x 100 mm), (7-9 ml)
[60] 15053	10 ml probówka z pokrywką (16 x 106 mm) 10 ml tube with cap (16 x 106 mm)
[60] *	Sarstedt S-Monovette® (15 x 92 mm), (7,5; 8,2; 8,5 ml)
[60] *	Sarstedt S-Monovette® (15 x 75 mm), (4; 4,3; 5,5 ml)
[60] *	10 ml Thermo Nalgene® Oak Ridge (16 x 81,5 mm)
[60] 15046	14 ml probówka z pokrywką (16,8 x 113,7 mm), Sarstedt® 14 ml tube with cap (16,8 x 113,7 mm), Sarstedt®
[60] *	10 ml probówka szklana (16 x 100 mm) 10 ml glass tube (16 x 100 mm) RCF max.=4000 RPM max.=4574
14317	
[28] *	15 ml probówka z dnem stożkowym z zakrętką (17 x 120 mm), Falcon®; [15050], 15ml (17 x 120 mm) 15 ml tube, conical bottom, with cap (17 x 120 mm), Falcon®; [15050] 15ml Sarstedt®(17 x 120 mm)
14317+14324	
[28] *	5 ml probówka z korkiem wciskanym (17 x 54,2 mm), Eppendorf® 5 ml tube with snap cap (17 x 54,2 mm), Eppendorf®

* probówka niedostępna w ofercie MPW lub dostępny odpowiednik (np:[15050]), patrz kolumna z prawej
tube is not offered by MPW or equivalent is available (e.g. [15050]), see column on the right

A. Wyposażenie dodatkowe/Optional accessories

MPW-352/R/RH

[28]	*	5 ml probówka z korkiem zakręcanym (17 x 66 mm), Eppendorf® 5 ml tube with screw cap (17 x 66 mm), Eppendorf®
		14318
[104]	*	Sarstedt S-Monovette® (11 x 92 mm), (4,5; 5 ml)
[104]	*	Sarstedt S-Monovette® (11 x 66 mm), (1,6; 2; 2,7; 3; 3,1 ml)
[104]	*	7 ml probówka szklana (12 x 100 mm) 7 ml glass tube (12 x 100 mm) RCF max.=4000 RPM max.=4574
[104]	*	5 ml probówka szklana (12 x 75 mm) 5 ml glass tube (12 x 75 mm) RCF max.=4000 RPM max.=4574
[104]	*	5 ml probówka z korkiem (12 x 85 mm), Sarstedt® 5 ml tube with cap (12 x 85 mm), Sarstedt®
[104]	*	6 ml probówka z pokrywką (11,5 x 92 mm), Sarstedt® 6 ml tube with cap (11,5 x 92 mm), Sarstedt®
		14319
[28]	15055	30 ml probówka z pokrywką (25,4 x 103,2 mm) 30 ml tube with cap (25,4 x 103,2 mm)
[28]	*	28 ml Thermo Nalgene® Oak Ridge (25,4 x 101,8 mm)
[12]	15222	30 ml probówka z pokrywką (25 x 94mm), Sterilin® 30 ml tube with cap (25 x 94 mm), Sterilin®
[12]	15223	30 ml probówka z pokrywką (25 x 94 mm), Sterilin® 30 ml tube with cap (25 x 94 mm), Sterilin®
[28]	*	30 ml probówka z pokrywką (25,5 x 94 mm), Nalgene® 30 ml tube with cap (25,5 x 94 mm), Nalgene®
[28]	*	30 ml Thermo Nalgene® Oak Ridge (25,5 x 94,3 mm) 30 ml Thermo Nalgene® Oak Ridge (25,5 x 94,3 mm)
[28]	*	25 ml probówka szklana (25 x 100 mm) 25 ml glass tube (25 x 100 mm) RCF max.=4000 RPM max.=4574
		14320
[48]	15046	14 ml probówka z pokrywką (16,8 x 113,7 mm), Sarstedt® 14 ml tube with cap (16,8 x 113,7 mm), Sarstedt®
[48]	15053	10 ml probówka z pokrywką (16 x 106 mm) 10 ml tube with cap (16 x 106 mm)
[48]	*	BD Vacutainer® (16 x 100 mm), (2,5-11 ml)
[48]	*	Greiner Vacuette® (16 x 100 mm), (7-9 ml)
[48]	*	Sarstedt S-Monovette® (15 x 92 mm), (7,5; 8,2; 8,5 ml)
[48]	*	Sarstedt S-Monovette® (16 x 92 mm), (9; 10 ml)
[48]	15121	10 ml probówka z dnem okrągłym i pokrywką (17 x 70 mm) 10 ml tube, round bottom, with cap (17 x 70 mm)
[48]	*	Sarstedt S-Monovette® (15 x 75 mm), (4; 4,3; 5,5 ml)
[48]	*	10 ml Thermo Nalgene® Oak Ridge (16 x 81,5 mm)
[48]	*	15 ml Thermo Nalgene® (16 x 113 mm) 15 ml Thermo Nalgene® (16 x 113 mm)
[48]	*	13 ml probówka (16x100mm), Sarstedt® nr 62.515.006 13 ml tube (16 x 100 mm), Sarstedt® no. 62.515.006
[48]	*	10 ml probówka szklana (16 x 100 mm) 10 ml glass tube (16 x 100 mm) RCF max.=4000 RPM max.=4574
		14321
[16]	15051	50 ml Thermo Nalgene® Oak Ridge (28,8 x 106,7 mm) 50 ml Thermo Nalgene® Oak Ridge (28,8 x 106,7 mm)
[16]	*	50 ml probówka Advanced Oak Ridge (29x102 mm), Herolab® nr 25 32 11 50 ml tube, Advanced Oak Ridge (29 x 102 mm), Herolab® no. 25 32 11
		14322
[72]	*	2-1,5 ml probówka (10,8x41,8 mm), Eppendorf®; [15011], 2 ml (10,8x41,8 mm); [15128], 1,5ml (10,8x40,5 mm)
		14323
[4]	15440	200 ml butelka płaskodenna (56 x 112 mm), Herolab® nr 25 33 73 200 ml bottle, flat bottom (56 x 112 mm), Herolab® no. 25 33 73
		14325
[68]	*	BD Vacutainer® (13 x 75 mm), (1,6-5,3 ml)
[68]	*	Sarstedt S-Monovette® (13 x 90 mm), (4,9; 5,6 ml)
[68]	*	Greiner Vacuette® (13 x 100 mm), (3,5-6 ml)
[68]	*	BD Vacutainer® (13 x 100 mm), (4-7 ml)
[68]	*	Greiner Vacuette® (13 x 75 mm), (1-4,5 ml)
[68]	*	Sarstedt S-Monovette® (13 x 75 mm), (2,7; 3; 4,3 ml)
[68]	*	Sarstedt S-Monovette® (11 x 66 mm), (1,6; 2; 2,7; 3; 3,1 ml)
[68]	*	Sarstedt S-Monovette® (11 x 92 mm), (4,5; 5 ml)
[68]	*	Sarstedt S-Monovette® (13 x 65 mm), (2,6; 2,9; 3,4; 3,8 ml)

* probówka niedostępna w ofercie MPW lub dostępny odpowiednik (np.[15050]), patrz kolumna z prawej
tube is not offered by MPW or equivalent is available (e.g. [15050]), see column on the right

A. Wyposażenie dodatkowe/Optional accessories

MPW-352/R/RH

- [68] * 5 ml probówka z korkiem (12 x 85 mm), Sarstedt®
5 ml tube with cap (12 x 85 mm), Sarstedt®
- [68] * 6 ml probówka z pokrywką (11,5 x 92 mm), Sarstedt®
6 ml tube with cap (11,5 x 92 mm), Sarstedt®

12436
RPM 5200 RCF 4807 Rmax 159 4 90

13042

14043

- [8] * 7 ml probówka szklana (12 x 100 mm)
7 ml glass tube (12 x 100 mm)
RCF max.=4000 RPM max.=4804
- [8] * 5 ml probówka szklana (12 x 75 mm)
5 ml glass tube (12 x 75 mm)
RCF max.=4000 RPM max.=4804

13045

14043

- [4] * 7 ml probówka szklana (12 x 100 mm)
7 ml glass tube (12 x 100 mm)
RCF max.=4000 RPM max.=4917
- [4] * 5 ml probówka szklana (12 x 75 mm)
5 ml glass tube (12 x 75 mm)
RCF max.=4000 RPM max.=4917

13437

14072

- [4] * 50 ml probówka szklana (35 x 100 mm)
50 ml glass tube (35 x 100 mm)
RCF max.=4000 RPM max.=4804

14106

- [28] * 7 ml probówka szklana (12 x 100 mm)
7 ml glass tube (12 x 100 mm)
RCF max.=4000 RPM max.=4804
- [28] * 5 ml probówka szklana (12 x 75 mm)
5 ml glass tube (12 x 75 mm)
RCF max.=4000 RPM max.=4804

14108

- [28] * 10 ml probówka szklana (16 x 100 mm)
10 ml glass tube (16 x 100 mm)
RCF max.=4000 RPM max.=4804

14109

- [28] * 7 ml probówka szklana (12 x 100 mm)
7 ml glass tube (12 x 100 mm)
RCF max.=4000 RPM max.=4804
- [28] * 5 ml probówka szklana (12 x 75 mm)
5 ml glass tube (12 x 75 mm)
RCF max.=4000 RPM max.=4804

14110

- [28] * 10 ml probówka szklana (16 x 100 mm)
10 ml glass tube (16 x 100 mm)
RCF max.=4000 RPM max.=4804

14111 NIE AUTOKLAWOWAĆ/DO NOT AUTOCLAVE

- [20] * 10 ml probówka szklana (16 x 100 mm)
10 ml glass tube (16 x 100 mm)
RCF max.=4000 RPM max.=4804

14197

- [4] * 100 ml probówka szklana (44 x 100 mm)
100 ml glass tube (44 x 100 mm)
RCF max.=4000 RPM max.=4804

14441

- [48] * 7 ml probówka szklana (12 x 100 mm)
7 ml glass tube (12 x 100 mm)
RCF max.=4000 RPM max.=4804

14446

- [48] * 7 ml probówka szklana (12 x 100 mm)
7 ml glass tube (12 x 100 mm)
RCF max.=4000 RPM max.=4804
- [48] * 5 ml probówka szklana (12 x 75 mm)
5 ml glass tube (12 x 75 mm)
RCF max.=4000 RPM max.=4804

A. Wyposażenie dodatkowe/Optional accessories
MPW-352/R/RH
13438+17111
14072

- [4] * 50 ml probówka szklana (35 x 100 mm)
 50 ml glass tube (35 x 100 mm)
 RCF max.=4000 RPM max.=4804

14106

- [28] * 7 ml probówka szklana (12 x 100 mm)
 7 ml glass tube (12 x 100 mm)
 RCF max.=4000 RPM max.=4804

- [28] * 5 ml probówka szklana (12 x 75 mm)
 5 ml glass tube (12 x 75 mm)
 RCF max.=4000 RPM max.=4804

14108

- [28] * 10 ml probówka szklana (16 x 100 mm)
 10 ml glass tube (16 x 100 mm)
 RCF max.=4000 RPM max.=4804

14109

- [28] * 7 ml probówka szklana (12 x 100 mm)
 7 ml glass tube (12 x 100 mm)
 RCF max.=4000 RPM max.=4804

- [28] * 5 ml probówka szklana (12 x 75 mm)
 5 ml glass tube (12 x 75 mm)
 RCF max.=4000 RPM max.=4804

14110

- [28] * 10 ml probówka szklana (16 x 100 mm)
 10 ml glass tube (16 x 100 mm)
 RCF max.=4000 RPM max.=4804

14111 NIE AUTOKLAWOWAĆ/DO NOT AUTOCLAVE

- [20] * 10 ml probówka szklana (16 x 100 mm)
 10 ml glass tube (16 x 100 mm)
 RCF max.=4000 RPM max.=4804

14197

- [4] * 100 ml probówka szklana (44 x 100 mm)
 100 ml glass tube (44 x 100 mm)
 RCF max.=4000 RPM max.=4804

14441

- [48] * 7 ml probówka szklana (12 x 100 mm)
 7 ml glass tube (12 x 100 mm)
 RCF max.=4000 RPM max.=4804

14446

- [48] * 7 ml probówka szklana (12 x 100 mm)
 7 ml glass tube (12 x 100 mm)
 RCF max.=4000 RPM max.=4804

- [48] * 5 ml probówka szklana (12 x 75 mm)
 5 ml glass tube (12 x 75 mm)
 RCF max.=4000 RPM max.=4804

13593
14190+14188

- [4] * 25 ml probówka szklana (25 x 100 mm)
 25 ml glass tube (25 x 100 mm)
 RCF max.=4000 RPM max.=4804

14181

- [20] * 7 ml probówka szklana (12 x 100 mm)
 7 ml glass tube (12 x 100 mm)
 RCF max.=4000 RPM max.=4804

- [20] * 5 ml probówka szklana (12 x 75 mm)
 5 ml glass tube (12 x 75 mm)
 RCF max.=4000 RPM max.=4804

14186

- [16] * 7 ml probówka szklana (12 x 100 mm)
 7 ml glass tube (12 x 100 mm)
 RCF max.=4000 RPM max.=4804

- [16] * 5 ml probówka szklana (12 x 75 mm)
 5 ml glass tube (12 x 75 mm)
 RCF max.=4000 RPM max.=4804

14187

- [16] * 10 ml probówka szklana (16 x 100 mm)
 10 ml glass tube (16 x 100 mm)
 RCF max.=4000 RPM max.=4804

A. Wyposażenie dodatkowe/Optional accessories

MPW-352/R/RH

14188

- [4] * 100 ml probówka szklana (44 x 100 mm)
 100 ml glass tube (44 x 100 mm)
 RCF max.=4000 RPM max.=4804

14192+14188

- [4] * 50 ml probówka szklana (35 x 100 mm)
 50 ml glass tube (35 x 100 mm)
 RCF max.=4000 RPM max.=4804

13042 R max 155 RCF 4686

14089 Rmax 155 RCF 4686

- [8] * 15 ml probówka z dnem stożkowym z zakrętką (17 x 120 mm), Falcon®; [15050], 15ml (17 x 120 mm)
 15 ml tube, conical bottom, with cap (17 x 120 mm), Falcon®; [15050] 15ml Sarstedt®(17 x 120 mm)
 bez wkładki/without adapter Rmax 155 RCF 4686

- [8] * 50 ml probówka z dnem stożkowym z zakrętką (30 x 117 mm), Falcon®; [15052] 50ml (30 x 117mm)
 50 ml tube, conical bottom, with cap (30 x 117 mm), Falcon®; [15052] 50ml Sarstedt® (30 x 117 mm)

- [8] * 50 ml probówka z dnem stożkowym bez rantu (30 x 115 mm), Greiner®
 50 ml tube, conical bottom, without skirt (30 x 115 mm), Greiner®

13045 R max 148 RCF 4474

14043 Rmax 148 RCF 4474

- [4] * Greiner Vacutette® (13 x 75 mm), (1-4,5 ml)

14089 Rmax 148 RCF 4474

- [4] * 15 ml probówka z dnem stożkowym z zakrętką (17 x 120 mm), Falcon®; [15050], 15ml (17 x 120 mm)
 15 ml tube, conical bottom, with cap (17 x 120 mm), Falcon®; [15050] 15ml Sarstedt®(17 x 120 mm)
 bez wkładki/without adapter Rmax 148 RCF 4474

- [4] * 50 ml probówka z dnem stożkowym z zakrętką (30 x 117 mm), Falcon®; [15052] 50ml (30 x 117mm)
 50 ml tube, conical bottom, with cap (30 x 117 mm), Falcon®; [15052] 50ml Sarstedt® (30 x 117 mm)

- [4] * 50 ml probówka z dnem stożkowym bez rantu (30 x 115 mm), Greiner®
 50 ml tube, conical bottom, without skirt (30 x 115 mm), Greiner®

13437 R max 155 RCF 4686

bez wkładki/without adapter Rmax 155 RCF 4686

- [4] 15440 200 ml butelka płaskodenna (56 x 112 mm), Herolab® nr 25 33 73
 200 ml bottle, flat bottom (56 x 112 mm), Herolab® no. 25 33 73

14106 Rmax 155 RCF 4686

- [28] * BD Vacutainer® (13 x 100 mm), (4-7 ml)
 [28] * Greiner Vacutette® (13 x 75 mm), (1-4,5 ml)
 [28] * Greiner Vacutette® (13 x 100 mm), (3,5-6 ml)
 [28] * Sarstedt S-Monovette® (13 x 75 mm), (2,7; 3; 4,3 ml)
 [28] * Sarstedt S-Monovette® (11 x 92 mm), (4,5; 5 ml)
 [28] * Sarstedt S-Monovette® (13 x 90 mm), (4,9; 5,6 ml)
 [28] * 5 ml probówka z korkiem (12 x 85 mm), Sarstedt®
 5 ml tube with cap (12 x 85 mm), Sarstedt®
 [28] * 6 ml probówka z pokrywką (11,5 x 92 mm), Sarstedt®
 6 ml tube with cap (11,5 x 92 mm), Sarstedt®

14108 Rmax 155 RCF 4686

- [28] 15053 10 ml probówka z pokrywką (16 x 106 mm)
 10 ml tube with cap (16 x 106 mm)
 [28] * BD Vacutainer® (16 x 100 mm), (2,5-11 ml)
 [28] * Greiner Vacutette® (16 x 100 mm), (7-9 ml)
 [28] * Sarstedt S-Monovette® (15 x 75 mm), (4; 4,3; 5,5 ml)
 [28] * Sarstedt S-Monovette® (15 x 92 mm), (7,5; 8,2; 8,5 ml)
 [28] * 10 ml Thermo Nalgene® Oak Ridge (16 x 81,5 mm)
 [28] * 15 ml Thermo Nalgene® (16 x 113 mm)
 15 ml Thermo Nalgene® (16 x 113 mm)

14109 Rmax 155 RCF 4686

- [28] * BD Vacutainer® (13 x 100 mm), (4-7 ml)
 [28] * Greiner Vacutette® (13 x 75 mm), (1-4,5 ml)
 [28] * Greiner Vacutette® (13 x 100 mm), (3,5-6 ml)
 [28] * Sarstedt S-Monovette® (13 x 75 mm), (2,7; 3; 4,3 ml)
 [28] * Sarstedt S-Monovette® (11 x 92 mm), (4,5; 5 ml)
 [28] * Sarstedt S-Monovette® (13 x 90 mm), (4,9; 5,6 ml)
 [28] * BD Vacutainer® (13 x 75 mm), (1,6-5,3 ml)
 [28] * Sarstedt S-Monovette® (11 x 66 mm), (1,6; 2; 2,7; 3; 3,1 ml)
 [28] * Sarstedt S-Monovette® (13 x 65 mm), (2,6; 2,9; 3,4; 3,8 ml)
 [28] * 5 ml probówka z korkiem (12 x 85 mm), Sarstedt®
 5 ml tube with cap (12 x 85 mm), Sarstedt®
 [28] * 6 ml probówka z pokrywką (11,5 x 92 mm), Sarstedt®
 6 ml tube with cap (11,5 x 92 mm), Sarstedt®

14110 Rmax 155 RCF 4686

* probówka niedostępna w ofercie MPW lub dostępny odpowiednik (np.[15050]), patrz kolumna z prawej
 tube is not offered by MPW or equivalent is available (e.g. [15050]), see column on the right

A. Wyposażenie dodatkowe/Optional accessories

MPW-352/R/RH

[28]	15053	10 ml probówka z pokrywką (16 x 106 mm) 10 ml tube with cap (16 x 106 mm)
[28]	*	BD Vacutainer® (16 x 100 mm), (2,5-11 ml)
[28]	*	Greiner Vacuette® (16 x 100 mm), (7-9 ml)
[28]	*	10 ml Thermo Nalgene® Oak Ridge (16 x 81,5 mm)
[28]	15046	14 ml probówka z pokrywką (16,8 x 113,7 mm), Sarstedt® 14 ml tube with cap (16,8 x 113,7 mm), Sarstedt®
[28]	*	15 ml Thermo Nalgene® (16 x 113 mm) 15 ml Thermo Nalgene® (16 x 113 mm)
		14111 NIE AUTOKLAWOWAĆ/DO NOT AUTOCLAVE Rmax 155 RCF 4686
[20]	15053	10 ml probówka z pokrywką (16 x 106 mm) 10 ml tube with cap (16 x 106 mm)
[20]	*	Sarstedt S-Monovette® (15 x 75 mm), (4; 4,3; 5,5 ml)
[20]	*	10 ml Thermo Nalgene® Oak Ridge (16 x 81,5 mm)
[20]	*	13 ml probówka (16x100mm), Sarstedt® nr 62.515.006 13 ml tube (16 x 100 mm), Sarstedt® no. 62.515.006
		14113 Rmax 155 RCF 4686
[4]	15051	50 ml Thermo Nalgene® Oak Ridge (28,8 x 106,7 mm) 50 ml Thermo Nalgene® Oak Ridge (28,8 x 106,7 mm)
[4]	*	50 ml probówka z dnem stożkowym z zakrętką (30 x 117 mm), Falcon®; [15052] 50ml (30 x 117mm) 50 ml tube, conical bottom, with cap (30 x 117 mm), Falcon®; [15052] 50ml Sarstedt® (30 x 117 mm)
[4]	*	50 ml probówka z dnem stożkowym bez rantu (30 x 115 mm), Greiner® 50 ml tube, conical bottom, without skirt (30 x 115 mm), Greiner®
		14197 Rmax 155 RCF 4686
[4]	15040	100 ml probówka z pokrywką (45,2 x 103,7 mm) 100 ml tube with cap (45,2 x 103,7 mm)
		14446 Rmax 155 RCF 4686
[48]	*	Sarstedt S-Monovette® (11 x 92 mm), (4,5; 5 ml)
[48]	*	Sarstedt S-Monovette® (11 x 66 mm), (1,6; 2; 2,7; 3; 3,1 ml)
[48]	*	5 ml probówka z korkiem (12 x 85 mm), Sarstedt® 5 ml tube with cap (12 x 85 mm), Sarstedt®
[48]	*	6 ml probówka z pokrywką (11,5 x 92 mm), Sarstedt® 6 ml tube with cap (11,5 x 92 mm), Sarstedt®
		14447 Rmax 155 RCF 4686
[48]	*	Sarstedt S-Monovette® (8 x 66 mm), (1,1; 1,2; 1,4 ml) Sarstedt S-Monovette® (8 x 66 mm), (1,1; 1,2; 1,4 ml)
		14449 Rmax 155 RCF 4686
[16]	15053	10 ml probówka z pokrywką (16 x 106 mm) 10 ml tube with cap (16 x 106 mm)
[16]	*	BD Vacutainer® (16 x 100 mm), (2,5-11 ml)
[16]	*	Sarstedt S-Monovette® (16 x 92 mm), (9; 10 ml)
[16]	*	13 ml probówka (16x100mm), Sarstedt® nr 62.515.006 13 ml tube (16 x 100 mm), Sarstedt® no. 62.515.006
		14450 Rmax 155 RCF 4686
[32]	*	2-1,5 ml probówka (10,8x41,8 mm), Eppendorf®; [15011], 2 ml (10,8x41,8 mm); [15128], 1,5ml (10,8x40,5 mm)
		13593 R max 155 RCF 4686
		14024 Rmax 155 RCF 4686
[4]	*	15 ml probówka z dnem stożkowym z zakrętką (17 x 120 mm), Falcon®; [15050], 15ml (17 x 120 mm) 15 ml tube, conical bottom, with cap (17 x 120 mm), Falcon®; [15050] 15ml Sarstedt®(17 x 120 mm)
		14181 Rmax 155 RCF 4686
[20]	*	Sarstedt S-Monovette® (11 x 66 mm), (1,6; 2; 2,7; 3; 3,1 ml)
[20]	*	Sarstedt S-Monovette® (11 x 92 mm), (4,5; 5 ml)
[20]	*	5 ml probówka z korkiem (12 x 85 mm), Sarstedt® 5 ml tube with cap (12 x 85 mm), Sarstedt®
[20]	*	6 ml probówka z pokrywką (11,5 x 92 mm), Sarstedt® 6 ml tube with cap (11,5 x 92 mm), Sarstedt®
		14186 Rmax 155 RCF 4686
[16]	*	BD Vacutainer® (13 x 75 mm), (1,6-5,3 ml)
[16]	*	BD Vacutainer® (13 x 100 mm), (4-7 ml)
[16]	*	Greiner Vacuette® (13 x 75 mm), (1-4,5 ml)
[16]	*	Greiner Vacuette® (13 x 100 mm), (3,5-6 ml)
[16]	*	Sarstedt S-Monovette® (11 x 66 mm), (1,6; 2; 2,7; 3; 3,1 ml)
[16]	*	Sarstedt S-Monovette® (13 x 65 mm), (2,6; 2,9; 3,4; 3,8 ml)
[16]	*	Sarstedt S-Monovette® (13 x 75 mm), (2,7; 3; 4,3 ml)
[16]	*	Sarstedt S-Monovette® (11 x 92 mm), (4,5; 5 ml)
[16]	*	Sarstedt S-Monovette® (13 x 90 mm), (4,9; 5,6 ml)
[16]	*	5 ml probówka z korkiem (12 x 85 mm), Sarstedt® 5 ml tube with cap (12 x 85 mm), Sarstedt®

* probówka niedostępna w ofercie MPW lub dostępny odpowiednik (np:[15050]), patrz kolumna z prawej
tube is not offered by MPW or equivalent is available (e.g. [15050]), see column on the right

A. Wyposażenie dodatkowe/Optional accessories

MPW-352/R/RH

[16] *	6 ml probówka z pokrywką (11,5 x 92 mm), Sarstedt® 6 ml tube with cap (11,5 x 92 mm), Sarstedt®
14187 Rmax 155 RCF 4686	
[16] 15053	10 ml probówka z pokrywką (16 x 106 mm) 10 ml tube with cap (16 x 106 mm)
[16] *	BD Vacutainer® (16 x 100 mm), (2,5-11 ml)
[16] *	Sarstedt S-Monovette® (15 x 92 mm), (7,5; 8,2; 8,5 ml)
[16] 15046	14 ml probówka z pokrywką (16,8 x 113,7 mm), Sarstedt® 14 ml tube with cap (16,8 x 113,7 mm), Sarstedt®
[16] *	Greiner Vacutette® (16 x 100 mm), (7-9 ml)
[16] *	Sarstedt S-Monovette® (15 x 75 mm), (4; 4,3; 5,5 ml)
[16] *	10 ml Thermo Nalgene® Oak Ridge (16 x 81,5 mm)
[16] *	15 ml Thermo Nalgene® (16 x 113 mm) 15 ml Thermo Nalgene® (16 x 113 mm)
14188 Rmax 155 RCF 4686	
[4] 15040	100 ml probówka z pokrywką (45,2 x 103,7 mm) 100 ml tube with cap (45,2 x 103,7 mm)
14194 Rmax 155 RCF 4686	
[12] *	2-1,5 ml probówka (10,8x41,8 mm), Eppendorf®; [15011], 2 ml (10,8x41,8 mm); [15128], 1,5ml (10,8x40,5 mm)
14189+14188 Rmax 155 RCF 4686	
[4] 15051	50 ml Thermo Nalgene® Oak Ridge (28,8 x 106,7 mm) 50 ml Thermo Nalgene® Oak Ridge (28,8 x 106,7 mm)
[4] *	50 ml probówka z dnem stożkowym z zakrętką (30 x 117 mm), Falcon®; [15052] 50ml (30 x 117mm) 50 ml tube, conical bottom, with cap (30 x 117 mm), Falcon®; [15052] 50ml Sarstedt® (30 x 117 mm)
[4] *	50 ml probówka z dnem stożkowym bez rantu (30 x 115 mm), Greiner® 50 ml tube, conical bottom, without skirt (30 x 115 mm), Greiner®
14190+14188 Rmax 155 RCF 4686	
[4] 15055	30 ml probówka z pokrywką (25,4 x 103,2 mm) 30 ml tube with cap (25,4 x 103,2 mm)
14226 Rmax 155 RCF 4686	
[4] *	50 ml probówka z dnem stożkowym z rantem (30 x 115 mm), Greiner® 50 ml tube, conical bottom, skirted (30 x 115 mm), Greiner®
13438+17111 R max 155 RCF 4686	
bez wkładki/without adapter Rmax 155 RCF 4686	
[4] 15440	200 ml butelka płaskodenna (56 x 112 mm), Herolab® nr 25 33 73 200 ml bottle, flat bottom (56 x 112 mm), Herolab® no. 25 33 73
14106 Rmax 155 RCF 4686	
[28] *	BD Vacutainer® (13 x 100 mm), (4-7 ml)
[28] *	Greiner Vacutette® (13 x 75 mm), (1-4,5 ml)
[28] *	Greiner Vacutette® (13 x 100 mm), (3,5-6 ml)
[28] *	Sarstedt S-Monovette® (13 x 75 mm), (2,7; 3; 4,3 ml)
[28] *	Sarstedt S-Monovette® (11 x 92 mm), (4,5; 5 ml)
[28] *	Sarstedt S-Monovette® (13 x 90 mm), (4,9; 5,6 ml)
[28] *	5 ml probówka z korkiem (12 x 85 mm), Sarstedt® 5 ml tube with cap (12 x 85 mm), Sarstedt®
[28] *	6 ml probówka z pokrywką (11,5 x 92 mm), Sarstedt® 6 ml tube with cap (11,5 x 92 mm), Sarstedt®
14108 Rmax 155 RCF 4686	
[28] 15053	10 ml probówka z pokrywką (16 x 106 mm) 10 ml tube with cap (16 x 106 mm)
[28] *	BD Vacutainer® (16 x 100 mm), (2,5-11 ml)
[28] *	Greiner Vacutette® (16 x 100 mm), (7-9 ml)
[28] *	Sarstedt S-Monovette® (15 x 75 mm), (4; 4,3; 5,5 ml)
[28] *	Sarstedt S-Monovette® (15 x 92 mm), (7,5; 8,2; 8,5 ml)
[28] *	10 ml Thermo Nalgene® Oak Ridge (16 x 81,5 mm)
14109 Rmax 155 RCF 4686	
[28] *	BD Vacutainer® (13 x 100 mm), (4-7 ml)
[28] *	Greiner Vacutette® (13 x 75 mm), (1-4,5 ml)
[28] *	Greiner Vacutette® (13 x 100 mm), (3,5-6 ml)
[28] *	Sarstedt S-Monovette® (13 x 75 mm), (2,7; 3; 4,3 ml)
[28] *	Sarstedt S-Monovette® (11 x 92 mm), (4,5; 5 ml)
[28] *	Sarstedt S-Monovette® (13 x 90 mm), (4,9; 5,6 ml)
[28] *	BD Vacutainer® (13 x 75 mm), (1,6-5,3 ml)
[28] *	Sarstedt S-Monovette® (11 x 66 mm), (1,6; 2; 2,7; 3; 3,1 ml)
[28] *	Sarstedt S-Monovette® (13 x 65 mm), (2,6; 2,9; 3,4; 3,8 ml)
[28] *	5 ml probówka z korkiem (12 x 85 mm), Sarstedt® 5 ml tube with cap (12 x 85 mm), Sarstedt®
[28] *	6 ml probówka z pokrywką (11,5 x 92 mm), Sarstedt® 6 ml tube with cap (11,5 x 92 mm), Sarstedt®

* probówka niedostępna w ofercie MPW lub dostępny odpowiednik (np.: [15050]), patrz kolumna z prawej
tube is not offered by MPW or equivalent is available (e.g. [15050]), see column on the right

A. Wyposażenie dodatkowe/Optional accessories

MPW-352/R/RH

14110 Rmax 155 RCF 4686

- [28] 15053 10 ml probówka z pokrywką (16 x 106 mm)
10 ml tube with cap (16 x 106 mm)
- [28] * BD Vacutainer® (16 x 100 mm), (2,5-11 ml)
- [28] * Sarstedt S-Monovette® (15 x 75 mm), (4; 4,3; 5,5 ml)
- [28] * Sarstedt S-Monovette® (15 x 92 mm), (7,5; 8,2; 8,5 ml)
- [28] * 10 ml Thermo Nalgene® Oak Ridge (16 x 81,5 mm)
- [28] 15046 14 ml probówka z pokrywką (16,8 x 113,7 mm), Sarstedt®
14 ml tube with cap (16,8 x 113,7 mm), Sarstedt®

14111 NIE AUTOKLAWOWAĆ/DO NOT AUTOCLAVE Rmax 155 RCF 4686

- [20] 15053 10 ml probówka z pokrywką (16 x 106 mm)
10 ml tube with cap (16 x 106 mm)
- [20] * Sarstedt S-Monovette® (15 x 75 mm), (4; 4,3; 5,5 ml)
- [20] * 10 ml Thermo Nalgene® Oak Ridge (16 x 81,5 mm)
- [20] * 13 ml probówka (16x100mm), Sarstedt® nr 62.515.006
13 ml tube (16 x 100 mm), Sarstedt® no. 62.515.006

14113 Rmax 155 RCF 4686

- [4] 15051 50 ml Thermo Nalgene® Oak Ridge (28,8 x 106,7 mm)
50 ml Thermo Nalgene® Oak Ridge (28,8 x 106,7 mm)
- [4] * 50 ml probówka z dnem stożkowym z zakrętką (30 x 117 mm), Falcon®; [15052] 50ml (30 x 117mm)
50 ml tube, conical bottom, with cap (30 x 117 mm), Falcon®; [15052] 50ml Sarstedt® (30 x 117 mm)
- [4] * 50 ml probówka z dnem stożkowym bez rantu (30 x 115 mm), Greiner®
50 ml tube, conical bottom, without skirt (30 x 115 mm), Greiner®

14197 Rmax 155 RCF 4686

- [4] 15040 100 ml probówka z pokrywką (45,2 x 103,7 mm)
100 ml tube with cap (45,2 x 103,7 mm)

14446 Rmax 155 RCF 4686

- [48] * Sarstedt S-Monovette® (11 x 92 mm), (4,5; 5 ml)
- [48] * Sarstedt S-Monovette® (11 x 66 mm), (1,6; 2; 2,7; 3; 3,1 ml)
- [48] * 5 ml probówka z korkiem (12 x 85 mm), Sarstedt®
5 ml tube with cap (12 x 85 mm), Sarstedt®
- [48] * 6 ml probówka z pokrywką (11,5 x 92 mm), Sarstedt®
6 ml tube with cap (11,5 x 92 mm), Sarstedt®

14447 Rmax 155 RCF 4686

- [48] * Sarstedt S-Monovette® (8 x 66 mm), (1,1; 1,2; 1,4 ml)
Sarstedt S-Monovette® (8 x 66 mm), (1,1; 1,2; 1,4 ml)

14449 Rmax 155 RCF 4686

- [16] 15053 10 ml probówka z pokrywką (16 x 106 mm)
10 ml tube with cap (16 x 106 mm)
- [16] * Sarstedt S-Monovette® (15 x 92 mm), (7,5; 8,2; 8,5 ml)
- [16] * Sarstedt S-Monovette® (16 x 92 mm), (9; 10 ml)
- [16] * Sarstedt S-Monovette® (15 x 75 mm), (4; 4,3; 5,5 ml)
- [16] * 13 ml probówka (16x100mm), Sarstedt® nr 62.515.006
13 ml tube (16 x 100 mm), Sarstedt® no. 62.515.006

13044C

14082

- [16] * BD Vacutainer® (13 x 100 mm), (4-7 ml)
- [16] * Greiner Vacuette® (13 x 100 mm), (3,5-6 ml)
- [16] * Sarstedt S-Monovette® (11 x 92 mm), (4,5; 5 ml)
- [16] * 7 ml probówka szklana (12 x 100 mm)
7 ml glass tube (12 x 100 mm)
RCF max.=4000 RPM max.=4744

bez wkładki/without adapter

- [16] 15053 10 ml probówka z pokrywką (16 x 106 mm)
10 ml tube with cap (16 x 106 mm)
- [16] * 15 ml probówka z dnem stożkowym z zakrętką (17 x 120 mm), Falcon®; [15050], 15ml (17 x 120 mm)
15 ml tube, conical bottom, with cap (17 x 120 mm), Falcon®; [15050] 15ml Sarstedt®(17 x 120 mm)
- [16] * BD Vacutainer® (16 x 100 mm), (2,5-11 ml)
- [16] * Sarstedt S-Monovette® (15 x 92 mm), (7,5; 8,2; 8,5 ml)
- [16] * Sarstedt S-Monovette® (16 x 92 mm), (9; 10 ml)
- [16] * 13 ml probówka (16x100mm), Sarstedt® nr 62.515.006
13 ml tube (16 x 100 mm), Sarstedt® no. 62.515.006
- [16] * 10 ml probówka szklana (16 x 100 mm)
10 ml glass tube (16 x 100 mm)
RCF max.=4000 RPM max.=4744

14082+14815

- [16] * BD Vacutainer® (13 x 75 mm), (1,6-5,3 ml)
- [16] * Greiner Vacuette® (13 x 75 mm), (1-4,5 ml)
- [16] * Sarstedt S-Monovette® (11 x 66 mm), (1,6; 2; 2,7; 3; 3,1 ml)
- [16] * Sarstedt S-Monovette® (13 x 65 mm), (2,6; 2,9; 3,4; 3,8 ml)

* probówka niedostępna w ofercie MPW lub dostępny odpowiednik (np:[15050]), patrz kolumna z prawej
tube is not offered by MPW or equivalent is available (e.g. [15050]), see column on the right

A. Wyposażenie dodatkowe/Optional accessories

MPW-352/R/RH

- [16] * Sarstedt S-Monovette® (13 x 75 mm), (2,7; 3; 4,3 ml)
 [16] * 5 ml probówka szklana (12 x 75 mm)
 5 ml glass tube (12 x 75 mm)
 RCF max.=4000 RPM max.=4744
14815
 [16] * Sarstedt S-Monovette® (15 x 75 mm), (4; 4,3; 5,5 ml)
 [16] * 10 ml Thermo Nalgene® Oak Ridge (16 x 81,5 mm)
 [16] 15121 10 ml probówka z dnem okrągłym i pokrywką (17 x 70 mm)
 10 ml tube, round bottom, with cap (17 x 70 mm)

12451
 RPM 3000 RCF 1036 Rmax 103 ↗ 90

13307

bez wkładki/without adapter

- [2] * płytka titracyjna DWP 96/2000µl (127,8x85,5x44,1 mm)
 deepwell plate DWP 96/2000µl (127,8 x 85,5 x 44,1 mm)
 [6] * płytka titracyjna MTP 28,8ml (86x128x15/17,5 mm)
 microtiter plate MTP 28,8 ml (86 x 128 x 15/17,5 mm)

12452
 RPM 2500 RCF 769 Rmax 110 ↗ 90

13606

bez wkładki/without adapter

- [4] 16610 system cytologiczny MPW® 2,2ml
 cytological system MPW® 2,2 ml

12582
 RPM 3200 RCF 1809 Rmax 158 ↗ 90

13583

14181

- [20] * Sarstedt S-Monovette® (11 x 66 mm), (1,6; 2; 2,7; 3; 3,1 ml)
 [20] * 7 ml probówka szklana (12 x 100 mm)
 7 ml glass tube (12 x 100 mm)
 [20] * 5 ml probówka szklana (12 x 75 mm)
 5 ml glass tube (12 x 75 mm)
 [20] * 5 ml probówka z korkiem (12 x 85 mm), Sarstedt®
 5 ml tube with cap (12 x 85 mm), Sarstedt®
 [20] * 6 ml probówka z pokrywką (11,5 x 92 mm), Sarstedt®
 6 ml tube with cap (11,5 x 92 mm), Sarstedt®

14186

- [16] * BD Vacutainer® (13 x 75 mm), (1,6-5,3 ml)
 [16] * BD Vacutainer® (13 x 100 mm), (4-7 ml)
 [16] * Greiner Vacuette® (13 x 75 mm), (1-4,5 ml)
 [16] * Greiner Vacuette® (13 x 100 mm), (3,5-6 ml)
 [16] * Sarstedt S-Monovette® (11 x 66 mm), (1,6; 2; 2,7; 3; 3,1 ml)
 [16] * Sarstedt S-Monovette® (13 x 65 mm), (2,6; 2,9; 3,4; 3,8 ml)
 [16] * Sarstedt S-Monovette® (13 x 75 mm), (2,7; 3; 4,3 ml)
 [16] * Sarstedt S-Monovette® (11 x 92 mm), (4,5; 5 ml)
 [16] * Sarstedt S-Monovette® (13 x 90 mm), (4,9; 5,6 ml)
 [16] * 7 ml probówka szklana (12 x 100 mm)
 7 ml glass tube (12 x 100 mm)
 [16] * 5 ml probówka szklana (12 x 75 mm)
 5 ml glass tube (12 x 75 mm)
 [16] * 5 ml probówka z korkiem (12 x 85 mm), Sarstedt®
 5 ml tube with cap (12 x 85 mm), Sarstedt®
 [16] * 6 ml probówka z pokrywką (11,5 x 92 mm), Sarstedt®
 6 ml tube with cap (11,5 x 92 mm), Sarstedt®

14187

- [16] 15053 10 ml probówka z pokrywką (16 x 106 mm)
 10 ml tube with cap (16 x 106 mm)
 [16] * BD Vacutainer® (16 x 100 mm), (2,5-11 ml)
 [16] * Sarstedt S-Monovette® (15 x 92 mm), (7,5; 8,2; 8,5 ml)
 [16] 15046 14 ml probówka z pokrywką (16,8 x 113,7 mm), Sarstedt®
 14 ml tube with cap (16,8 x 113,7 mm), Sarstedt®
 [16] * Greiner Vacuette® (16 x 100 mm), (7-9 ml)
 [16] * Sarstedt S-Monovette® (15 x 75 mm), (4; 4,3; 5,5 ml)
 [16] * 15 ml Thermo Nalgene® (16 x 113 mm)
 15 ml Thermo Nalgene® (16 x 113 mm)
 [16] * 10 ml probówka szklana (16 x 100 mm)
 10 ml glass tube (16 x 100 mm)

14584

A. Wyposażenie dodatkowe/Optional accessories**MPW-352/R/RH**

[16] * BD Vacutainer® CPT™ (16 x 125 mm), (8 ml)

Suma końcowa



EU DECLARATION OF CONFORMITY

This EU declaration of conformity is issued under the sole responsibility of the manufacturer.

Manufacturer: "MPW MED. INSTRUMENTS" SPÓŁDZIELNIA PRACY
46 Boremlowska Street, 04-347 Warsaw, Poland

The Quality Management System complies with the standards: PN-EN ISO 9001:2015, PN-EN ISO 13485:2016

SRN: PL-MF-000032831

Device name: Laboratory centrifuge MPW-352
(with the accessory indicated in the operating instructions provided with the centrifuge)

BASIC UDI-DI: 590538636-IVD-CEN-009-6M

Catalogue numbers:	10352/2-56	10352/1-56	10352/1-56/100
	10352/1-56/110	10352/1-56/127	

The aforementioned device is in conformity with the following EU regulations and directives:

2017/746 (IVDR) REGULATION (EU) 2017/746 OF THE EUROPEAN PARLIAMENT AND OF THE COUNCIL of 5 April 2017 on in vitro diagnostic medical devices and repealing Directive 98/79/EC and Commission Decision 2010/227/EU, including the changes published prior to the date of this declaration.

2011/65/EU (RoHS 2) DIRECTIVE 2011/65/EU OF THE EUROPEAN PARLIAMENT AND OF THE COUNCIL of 8 June 2011 on the restriction of the use of certain hazardous substances in electrical and electronic equipment, including the changes published prior to the date of this declaration.

Intended purpose: The device is intended for the separation of the mixtures of the liquid substances derived from the human body, including blood, urine, and other body fluids, and for the preparation of the samples intended for further in vitro diagnostics procedures.

Risk class: Class A
(in accordance with the rule 5 of Annex VIII of Regulation (EU) 2017/746).

The conformity assessment of the device and accessory has been carried out in accordance with Article 48(10) of Regulation (EU) 2017/746.

Wojciech Anisiewicz
Vice-President of the Management Board

Warsaw, 23 January 2023

Lukasz Sałancki
President of the Management Board

no. 10.352.160.en



EU DECLARATION OF CONFORMITY

This EU declaration of conformity is issued under the sole responsibility of the manufacturer.

Manufacturer: "MPW MED. INSTRUMENTS" SPÓŁDZIELNIA PRACY
46 Boremlowska Street, 04-347 Warsaw, Poland

The Quality Management System complies with the standards: PN-EN ISO 9001:2015, PN-EN ISO 13485:2016

SRN: PL-MF-000032831

Device name: Refrigerated laboratory centrifuge MPW-352R
(with the accessory indicated in the operating instructions provided with the centrifuge)

BASIC UDI-DI: 590538636-IVD-CEN-002-5Y

Catalogue numbers: 10352R/2-5 10352R/2-6 10352R/1-6
10352R/1-6/100 10352R/1-6/110 10352R/1-6/127

The aforementioned device is in conformity with the following EU regulations and directives:

2017/746 (IVDR) REGULATION (EU) 2017/746 OF THE EUROPEAN PARLIAMENT AND OF THE COUNCIL of 5 April 2017 on in vitro diagnostic medical devices and repealing Directive 98/79/EC and Commission Decision 2010/227/EU, including the changes published prior to the date of this declaration.

2011/65/EU (RoHS 2) DIRECTIVE 2011/65/EU OF THE EUROPEAN PARLIAMENT AND OF THE COUNCIL of 8 June 2011 on the restriction of the use of certain hazardous substances in electrical and electronic equipment, including the changes published prior to the date of this declaration.

Intended purpose: The device is intended for the separation of the mixtures of the liquid substances derived from the human body, including blood, urine, and other body fluids, and for the preparation of the samples intended for further in vitro diagnostics procedures.

Risk class: Class A
(in accordance with the rule 5 of Annex VIII of Regulation (EU) 2017/746).

The conformity assessment of the device and accessory has been carried out in accordance with Article 48(10) of Regulation (EU) 2017/746.

Wojciech Anisiewicz
Vice-President of the Management Board

Łukasz Sałański
President of the Management Board



EU DECLARATION OF CONFORMITY

This EU declaration of conformity is issued under the sole responsibility of the manufacturer.

Manufacturer: "MPW MED. INSTRUMENTS" SPÓŁDZIELNIA PRACY
46 Boremlowska Street, 04-347 Warsaw, Poland

The Quality Management System complies with the standards: PN-EN ISO 9001:2015, PN-EN ISO 13485:2016

SRN: PL-MF-000032831

Device name: Refrigerated and heated laboratory centrifuge MPW-352RH
(with the accessory indicated in the operating instructions provided with the centrifuge)

BASIC UDI-DI: 590538636-IVD-CEN-010-5X

Catalogue numbers: 10352RH/2-5 10352RH/2-6 10352RH/1-6
10352RH/1-6/100 10352RH/1-6/110 10352RH/1-6/127

The aforementioned device is in conformity with the following EU regulations and directives:

2017/746 (IVDR) REGULATION (EU) 2017/746 OF THE EUROPEAN PARLIAMENT AND OF THE COUNCIL of 5 April 2017 on in vitro diagnostic medical devices and repealing Directive 98/79/EC and Commission Decision 2010/227/EU, including the changes published prior to the date of this declaration.

2011/65/EU (RoHS 2) DIRECTIVE 2011/65/EU OF THE EUROPEAN PARLIAMENT AND OF THE COUNCIL of 8 June 2011 on the restriction of the use of certain hazardous substances in electrical and electronic equipment, including the changes published prior to the date of this declaration.

Intended purpose: The device is intended for the separation of the mixtures of the liquid substances derived from the human body, including blood, urine, and other body fluids, and for the preparation of the samples intended for further in vitro diagnostics procedures.

Risk class: Class A
(in accordance with the rule 5 of Annex VIII of Regulation (EU) 2017/746).

The conformity assessment of the device and accessory has been carried out in accordance with Article 48(10) of Regulation (EU) 2017/746.

Wojciech Anisiewicz
Vice-President of the Management Board

Warsaw, 23 January 2023

Łukasz Sański
President of the Management Board

no. 10.352RH.16o.en

DECLARATION OF DECONTAMINATION

(repair)

In order to protect our employees please fill out the declaration of decontamination completely before sending centrifuge to the manufacturer (repair).

If it is impossible to completely and effectively decontaminate the device, it should be treated in accordance with the regulations for medical waste.

1. Device:

- type:
- serial No.:

2. Description of decontamination

(see user manual)

.....
.....
.....
.....

3. Decontamination carried out by:

name:

4. Date and signature:

.....

DECLARATION OF DECONTAMINATION

(return)

In order to protect our employees please fill out the declaration of decontamination completely before sending centrifuge to the manufacturer (return).

If it is impossible to completely and effectively decontaminate the device, it should be treated in accordance with the regulations for medical waste.

1. Device:

- type:
- serial No.:

2. Description of decontamination

(see user manual)

.....
.....
.....
.....

3. Decontamination carried out by:


name:

4. Date and signature:

.....

NOMOGRAM

Centrifuging radius [cm]

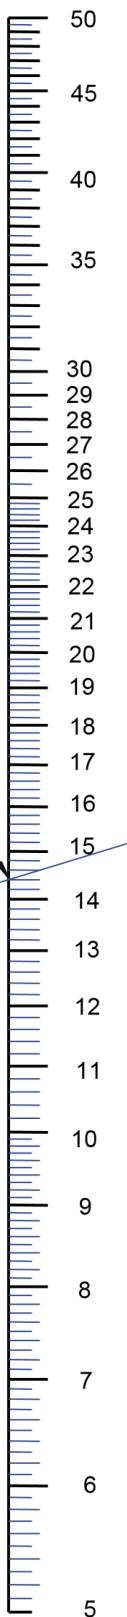


Formula used for calculation of this nomogram :

$$R.C.F. = 11,18 * r * (n/1000)^2$$


where :

- R.C.F. - multiple of gravitational acceleration
- r - centrifuging radius (cm)
- n - rotational speed (r.p.m.)
- g - gravitational acceleration

R.C.F. (x "g")
multiple of gravitational acceleration

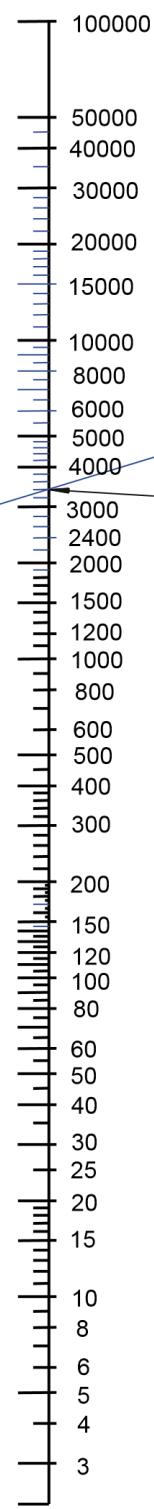

[r.p.m.]

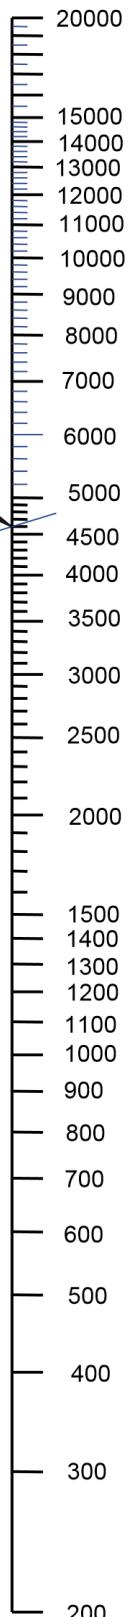

A

B

C

Example of making use
of the nomogram:

$$\begin{aligned} A &= 14,4 \text{ cm} \\ B &= 4600 \text{ r.p.m.} \\ C &= 3400 \times g \end{aligned}$$

$$n = 1000 * \sqrt{\frac{RCF}{(11,18 * r)}}$$

$$r = \left[\frac{RCF}{11,18 * \left(\frac{n}{1000} \right)^2} \right]$$